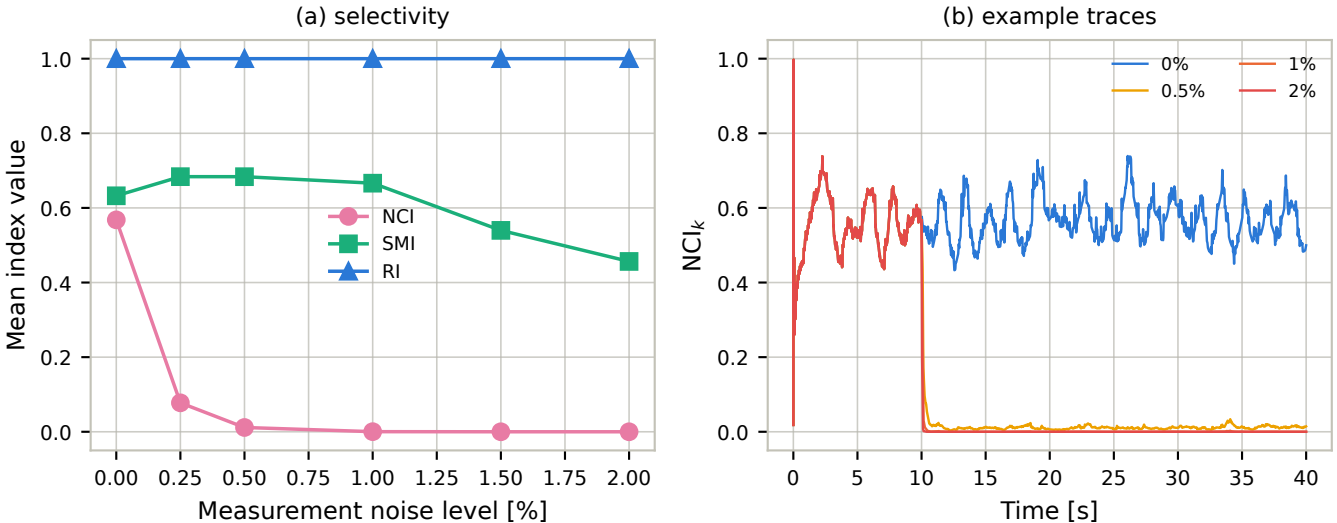S6: measurement-noise robustness of NCI