


SCRAG - measured metrics by module

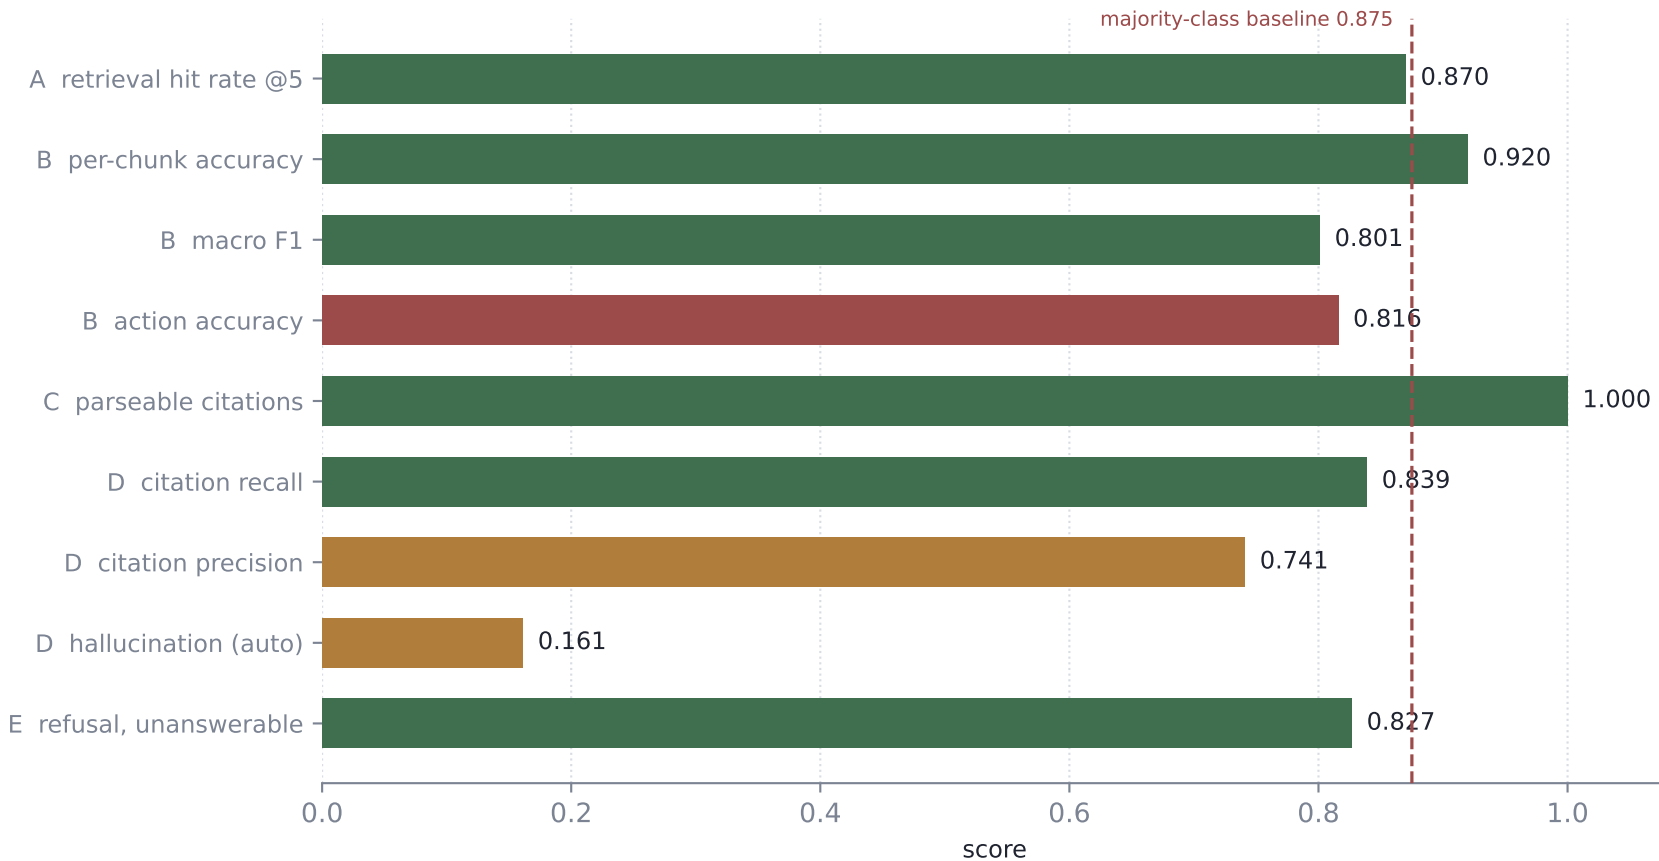

Hallucination rate is verifier-derived and an upper bound (docs/error-analysis.md). Faithfulness and the A-E ablation are absent: not measured.