


Certificate of Analysis

ISO GUIDE 34
ANAB Cert# AR-1470

ISO/IEC 17025
ANAB Cert# AT-1467

N 22-1

NAPHTHALENE CERTIFIED REFERENCE MATERIAL



CERTIFIED PURITY: 99.8%, $U_{\text{CRM}} = \pm 0.2\%$ $k = 2$
(Mass Balance/as is basis)

NOMINAL PACKAGE SIZE: 1g

CATALOG #: PHR1275

LOT #: LRAA9072

CERTIFICATE VERSION: LRAA9072.1

ISSUE DATE: 15 September 2015

Note: Certificates may be updated due to Pharmacopeial Lot changes or the availability of new data.

Check our website at: www.sigma-aldrich.com for the most current version.

CRM EXPIRATION: 31 December 2020 (Proper Storage and Handling Required).

RECEIPT DATE: _____

Note: this space is provided for convenience only and its use is not required.

STORAGE: Store at Room Temperature/Protect from Light, keep container tightly closed. Attachment of a 20 mm aluminum crimp seal recommended for unused portions.

CHEMICAL FORMULA: $C_{10}H_8$

MW: 128.2

PHYSICAL DESCRIPTION: White powder in amber vial **CAS #:** 91-20-3

HAZARDS: Read Safety Data Sheet before using. All chemical reference materials should be considered potentially hazardous and should be used only by qualified laboratory personnel.

SIGMA-ALDRICH



INSTRUCTIONS FOR USE: Do not dry, use on the as is basis. The internal pressure of the container may be slightly different from the atmospheric pressure at the user's location. Open slowly and carefully to avoid dispersion of the material. This material is intended for R&D use only. Not for drug, household or other uses.

TRACEABILITY ASSAY

Comparative assay demonstrates direct traceability to Pharmacopeial Standards

Specification: None

METHOD: HPLC

Column: Ascentis Express ES-CN, 4.6 x 100mm, 2.7µm

Mobile Phase: Water, Acetonitrile (40:60)

Flow Rate: 1mL/min

Column Temperature: 25°C

Injection: 5µL

Detector: 254nm

ASSAY vs. USP REFERENCE STANDARD (as is basis)

ASSAY VALUE


101.1%

vs. USP LOT

H0L124

Labeled Content = 1.00mg/mg

Representative Chromatogram from Lot: LRAA9072 Analysis

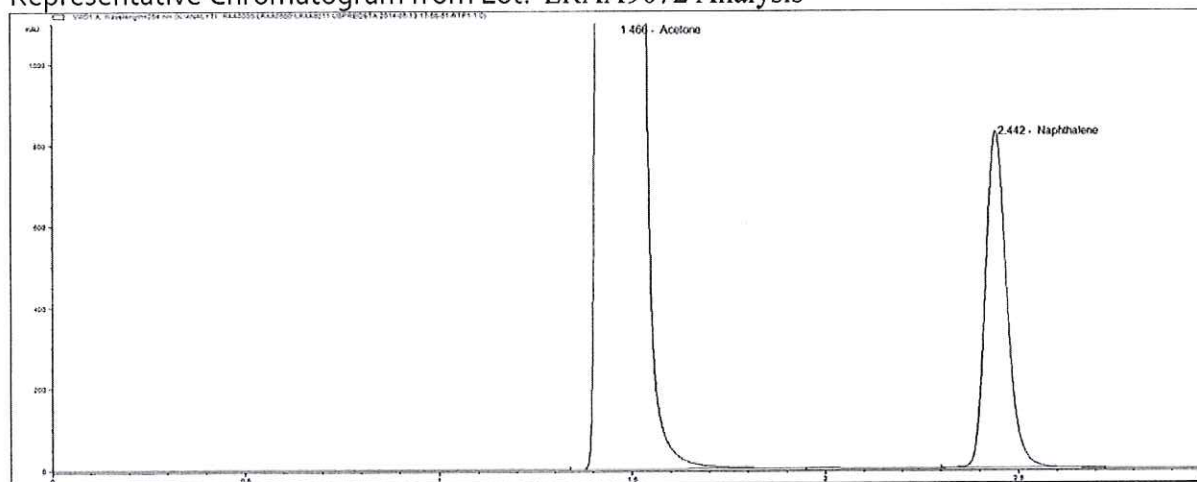

PURITY DETERMINATION BY MASS BALANCE

CHROMATOGRAPHIC IMPURITY ANALYSIS

METHOD: GC

Column: Equity 1, 30m x 0.25mm x 0.25 μ m

Carrier gas: H₂

Flow: 1.5mL/min

Split Ratio: Splitless


Injection/Temperature: 1 μ L/250°C

Temperature Program: 40°C for 5min, 7°C/min to 135°C, hold 5min, 20°C/min to 230°C, hold 3min

Detector/Temperature: FID, 250°C

Impurity 1: 0.1%

Representative Chromatogram from Lot: LRAA9072 Impurity Analysis

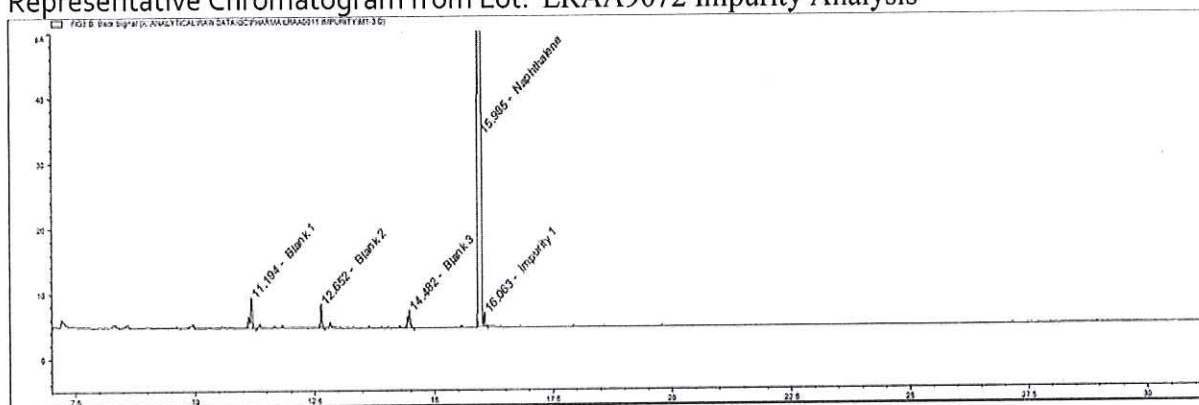

RESIDUAL SOLVENTS

Method: GC-MS Headspace (ref.: Residual Solvents <467>, USP34)

Column: DB-1301

Carrier gas: He

Flow: 1.2mL/min

Split Ratio: 1:5

Injection/Temperature: 1 μ L/250°C

Temperature Program: 40°C for 20min, 10°C/min to 240°C, hold 20min

Solvents Detected: None

WATER DETERMINATION

Method: Karl Fisher titration

Mean of three measurements, Water Content = 0.05%



RESIDUE ANALYSIS

Method: Sulfated Ash

Sample Size: ~1g


Mean of three measurements, Residue = **0.03%**

CERTIFIED PURITY BY MASS BALANCE [100% - Impurities (normalized)]

99.8% $U_{\text{crm}} = \pm 0.2\%$, $k = 2$
(as is basis)

IDENTIFICATION TESTS

INFRARED SPECTROPHOTOMETRY (Comparative identification analysis demonstrates direct traceability to Pharmacopeial standards)

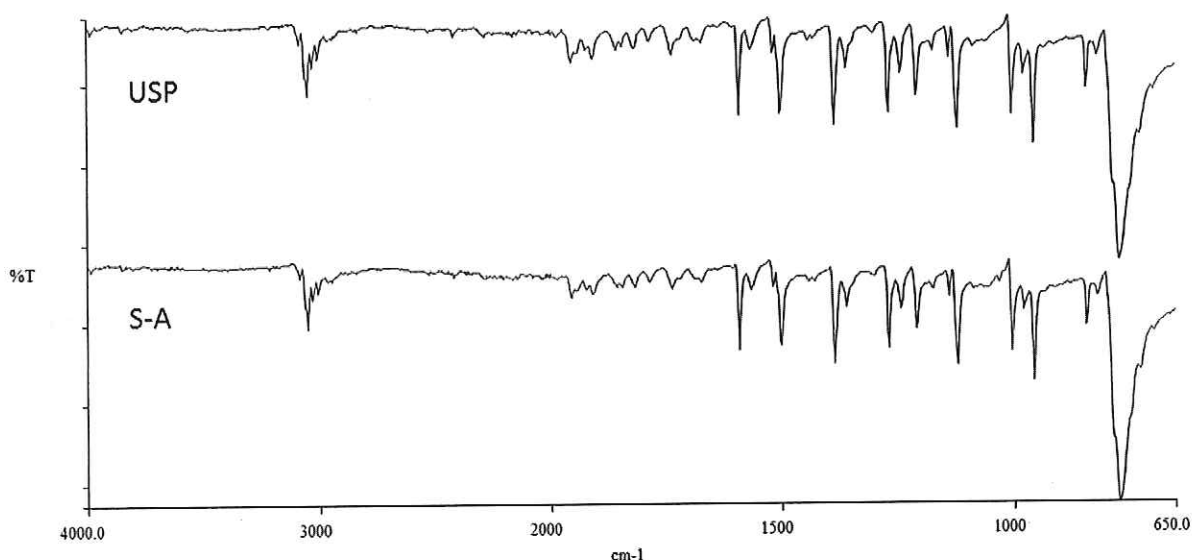


—— Naphthalene USP Lot H0L124
—— Naphthalene S-A Lot LRAA9072

PERKIN ELMER SPECTRUM 100
SAMPLING: UNIVERSAL ATR



¹H NMR (Data provided by an external laboratory; not in scope of accreditation)

LRAA9072 Naphthalene in CDCl₃

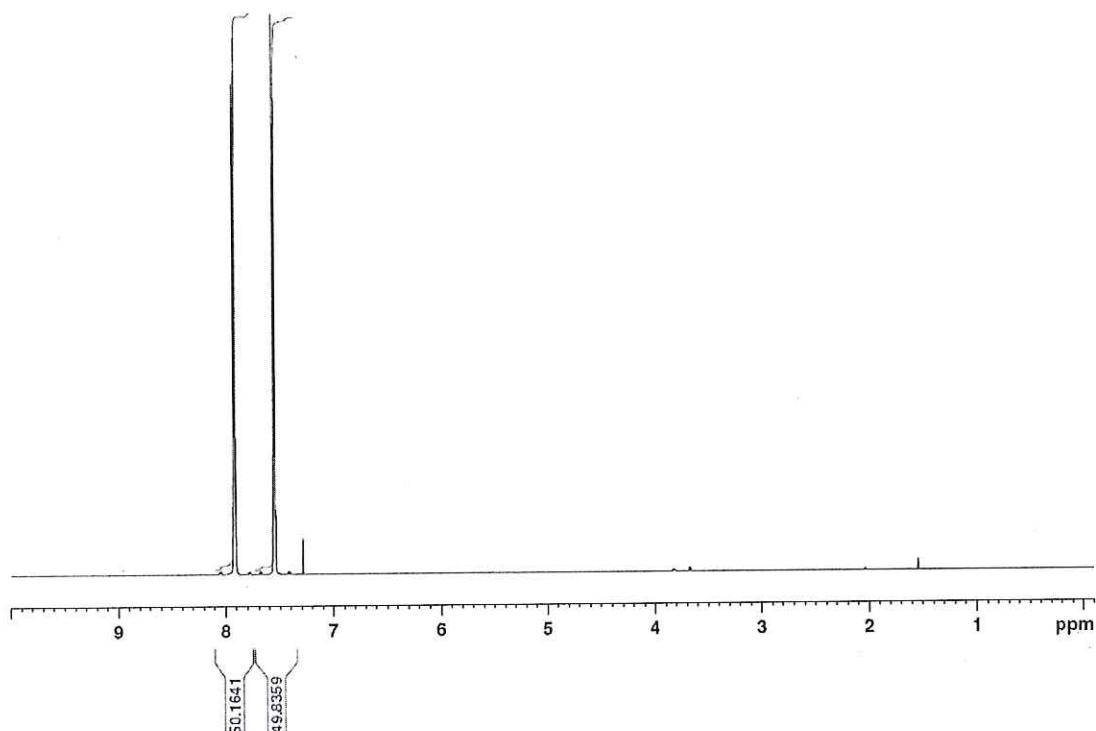

Consistent with structure

ELEMENTAL ANALYSIS (Data provided by an external laboratory; not in scope of accreditation)

Exeter Analytical 440 Elemental Analyzer

Combustion method

%	Theoretical	Result 1	Result 2	Mean
C	54.32	93.20	93.49	93.71
H	5.70	6.24	6.28	6.29

HOMOGENEITY ASSESSMENT

Homogeneity was assessed in accordance with ISO Guide 35. Completed units were sampled using a random stratified sampling protocol. The results of chemical analysis were then compared by Single Factor Analysis of Variance (ANOVA). The uncertainty due to homogeneity was derived from the ANOVA. Heterogeneity was not detected under the conditions of the ANOVA.

Analytical Method: HPLC

Sample size: ~60mg



UNCERTAINTY STATEMENT

Uncertainty values in this document are expressed as Expanded Uncertainty (U_{crm}) corresponding to the 95% confidence interval. U_{crm} is derived from the combined standard uncertainty multiplied by the coverage factor k , which is obtained from a t -distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies.

STABILITY ASSESSMENT

Significance of the stability assessment will be demonstrated if the analytical result of the study and the range of values represented by the Expanded Uncertainty do not overlap the result of the original assay and the range of its values represented by the Expanded Uncertainty. The method employed will usually be the same method used to characterize the assay value in the initial evaluation.

Long Term Stability Evaluation - An assessment, or re-test, versus a Compendial Reference Standard may be scheduled, within the 3 year anniversary date of a release of a Secondary Standard. The re-test interval will be determined on a case-by-case basis.

Short Term Stability Study - It is useful to assess stability under reasonably anticipated, short term transport conditions by simulating exposure of the product to humidity and temperature stress. This type of study is conducted under controlled conditions of elevated temperature and humidity.



Operations Manager



QA Supervisor

APPENDIX

Original Release Date: 15 September 2015

