Sea-Bird Scientific
13431 NE 20th Street
Bellevue, WA 98005
USA

+1 425-643-9866
seabird@seabird.com
www.seabird.com

SENSOR SERIAL NUMBER: 3765
CALIBRATION DATE: 23-Mar-26

SBE 37 PRESSURE CALIBRATION DATA
1450 psia S/N 5754

COEFFICIENTS:

PA0 =	5.778449e-01	PTCA0 =	-2.327268e+02
PA1 =	6.891542e-02	PTCA1 =	4.730162e-01
PA2 =	-5.405452e-09	PTCA2 =	-3.941180e-03
		PTCB0 =	2.476912e+01
		PTCB1 =	-7.750000e-04
		PTCB2 =	0.000000e+00

PRESSURE SPAN CALIBRATION

PRESSURE (PSIA)	INSTRUMENT OUTPUT (counts)	TEMPERATURE (°C)	COMPUTED PRESSURE (PSIA)	RESIDUAL (%FSR)
14.58	-20.1	21.6	14.66	0.01
301.66	4140.8	21.5	301.51	-0.01
588.22	8301.9	21.5	588.17	-0.00
875.52	12476.4	21.4	875.57	0.00
1162.79	16651.3	21.4	1162.81	0.00
1450.00	20827.2	21.3	1449.93	-0.00
1163.18	16657.2	21.3	1163.22	0.00
876.03	12484.0	21.3	876.10	0.00
588.89	8312.9	21.3	588.93	0.00
301.63	4141.6	21.3	301.56	-0.00
14.58	-20.7	21.4	14.63	0.00

THERMAL CORRECTION

TEMP (°C)	INSTRUMENT OUTPUT (counts)
32.50	-7.65
29.00	-8.28
24.00	-9.82
18.50	-11.26
15.00	-12.68
4.50	-16.78
1.00	-18.30

TEMPERATURE (°C)	SPAN
-5.00	24.77
35.00	24.74

x = instrument output - PTCA0 - PTCA1 * t - PTCA2 * t^2

n = x * PTCB0 / (PTCB0 + PTCB1 * t + PTCB2 * t^2)

pressure (PSIA) = PA0 + PA1 * n + PA2 * n^2

Residual (%FSR) = (computed pressure - true pressure) * 100 / Full Scale Range

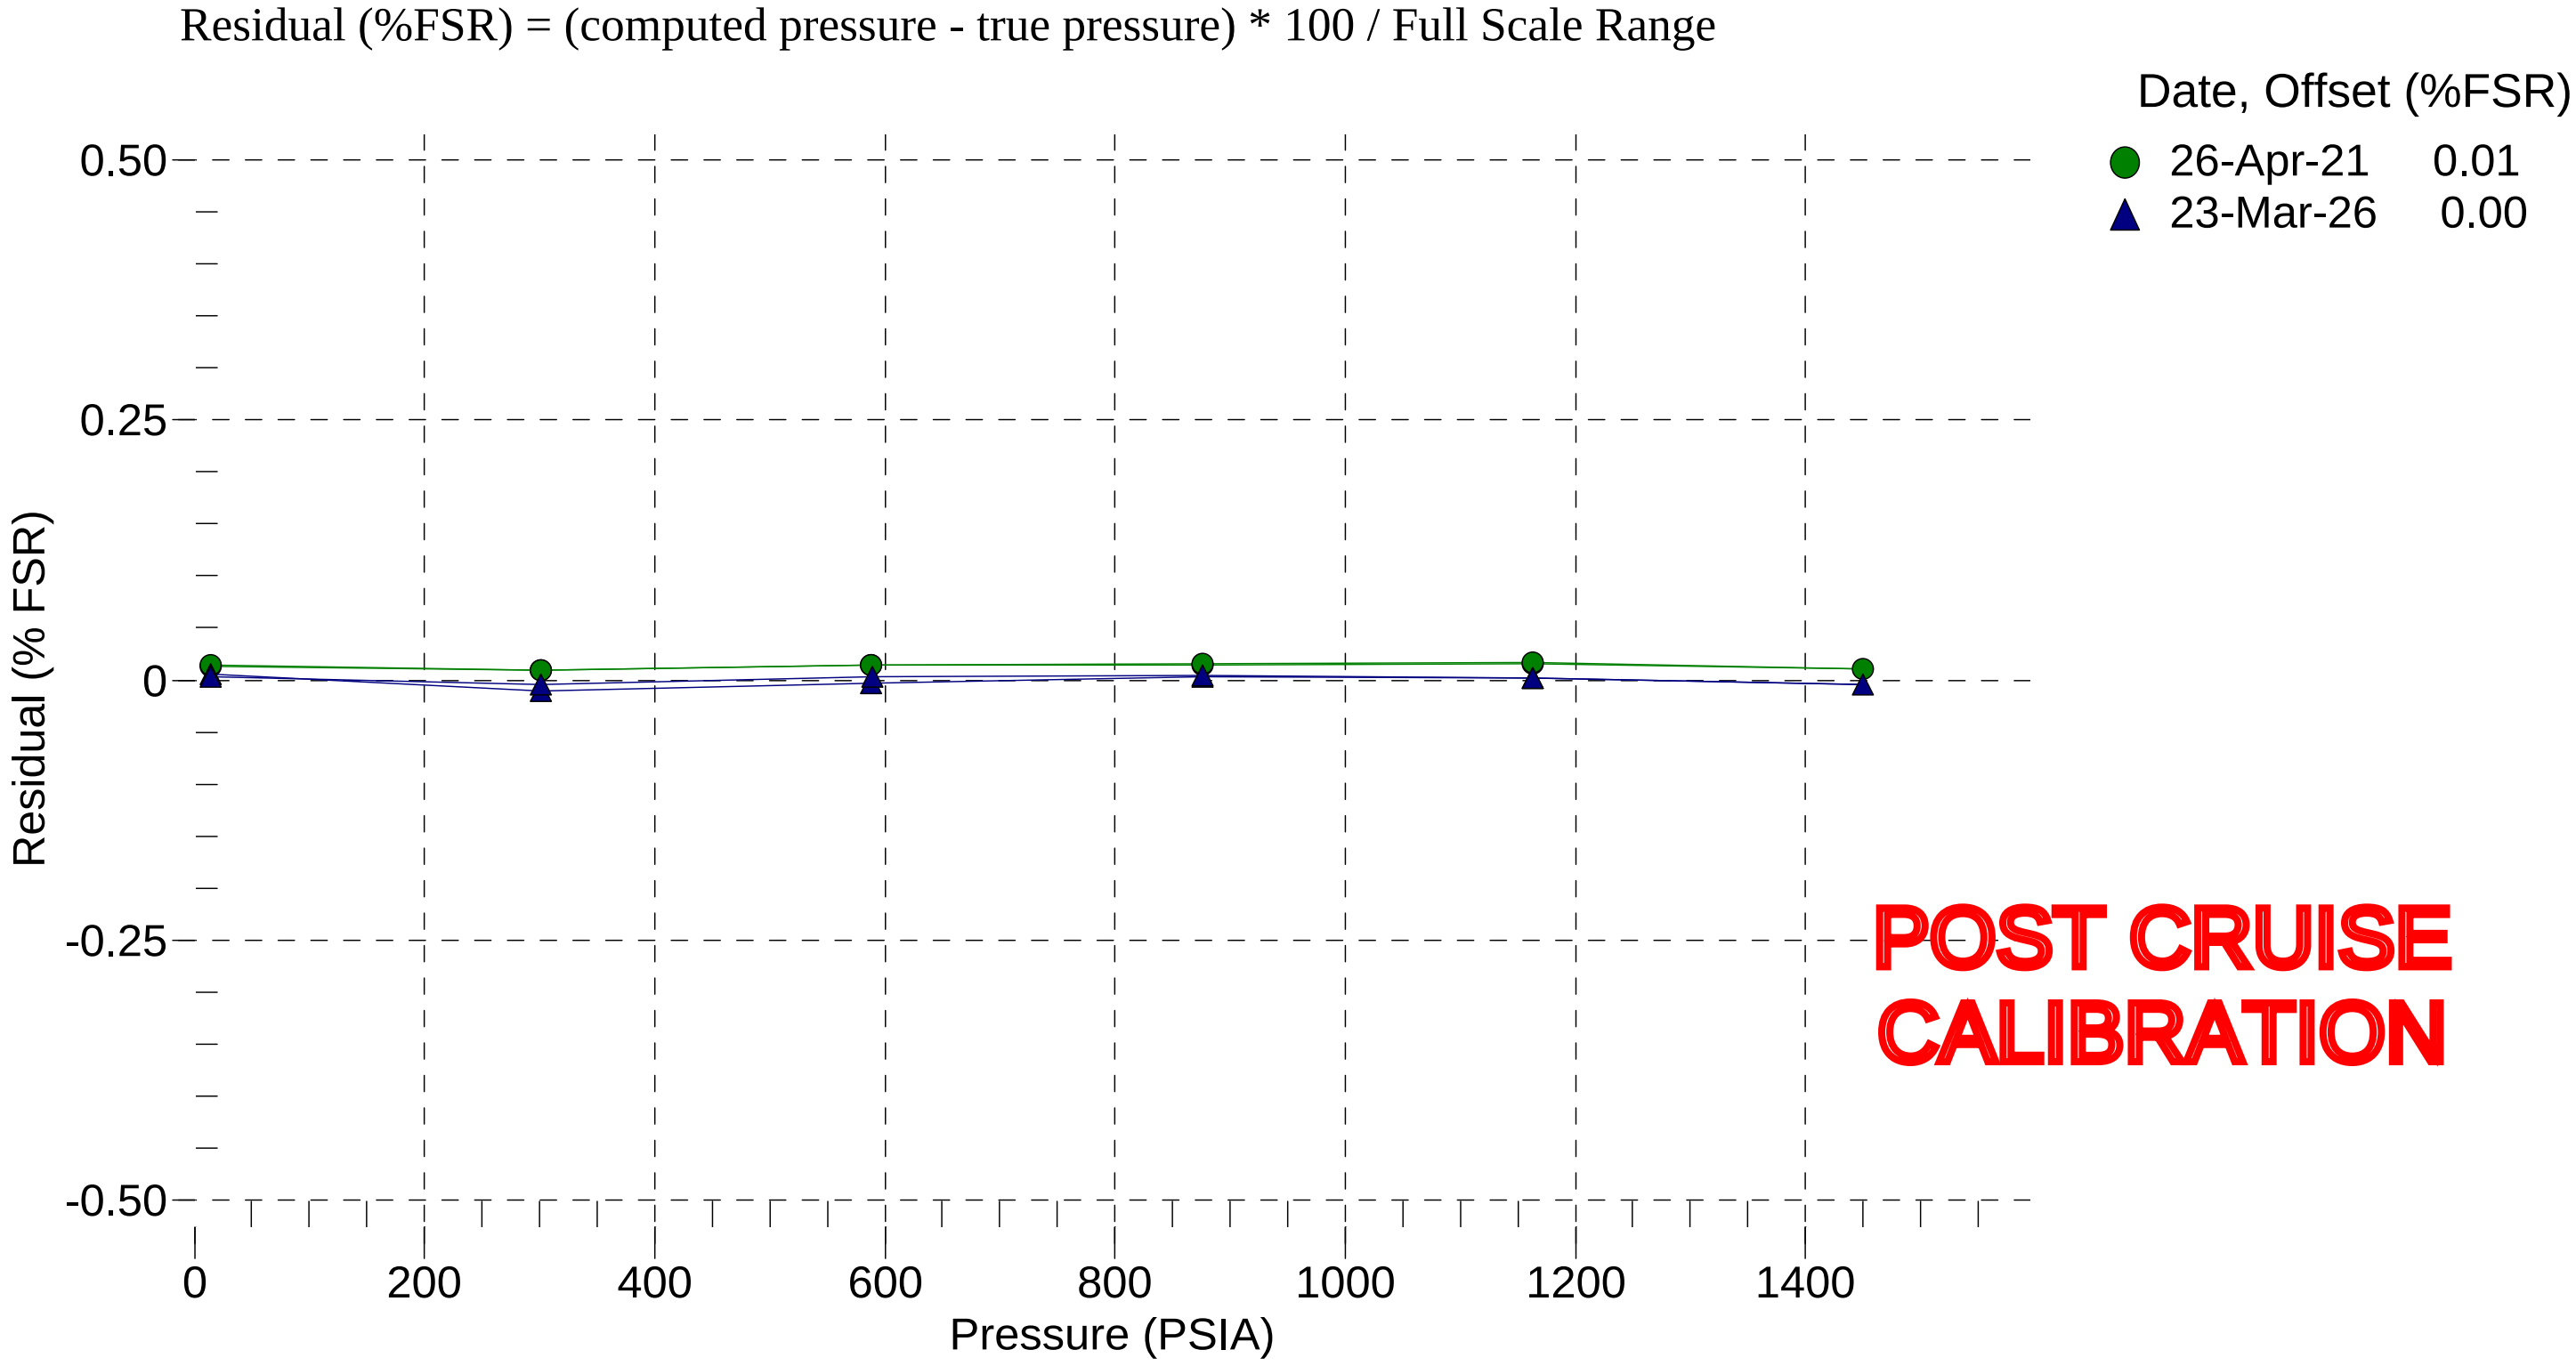

POST CRUISE CALIBRATION