Sea-Bird Scientific
13431 NE 20th Street
Bellevue, WA 98005
USA

+1 425-643-9866
seabird@seabird.com
www.seabird.com

SENSOR SERIAL NUMBER: 3765
CALIBRATION DATE: 24-Mar-26

SBE 37 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

```
g =  -1.026288e+00
h =   1.409858e-01
i =  -1.136649e-04
j =   2.960037e-05

CPcor = -9.5700e-008
CTcor =  3.2500e-006
WBOTC =  -8.7050e-06
```

BATH TEMP (° C)	BATH SAL (PSU)	BATH COND (S/m)	INSTRUMENT OUTPUT (Hz)	INSTRUMENT COND (S/m)	RESIDUAL (S/m)
22.0000	0.0000	0.00000	2699.16	0.00000	0.00000
0.9999	34.5698	2.95689	5310.97	2.95690	0.00001
4.5001	34.5504	3.26211	5509.99	3.26209	-0.00002
15.0000	34.5089	4.23787	6102.19	4.23789	0.00001
18.5000	34.4996	4.58087	6296.88	4.58087	0.00000
24.0000	34.4888	5.13527	6599.15	5.13525	-0.00001
29.0000	34.4808	5.65352	6869.42	5.65352	0.00001
32.5000	34.4732	6.02289	7055.60	6.02299	0.00010

f = Instrument Output(Hz) * sqrt(1.0 + WBOTC * t) / 1000.0

t = temperature (°C);   p = pressure (decibars); δ = CTcor; ε = CPcor;

Conductivity (S/m) = $(g + h * f^2 + i * f^3 + j * f^4) / (1 + \delta * t + \varepsilon * p)$

Residual (Siemens/meter) = instrument conductivity - bath conductivity

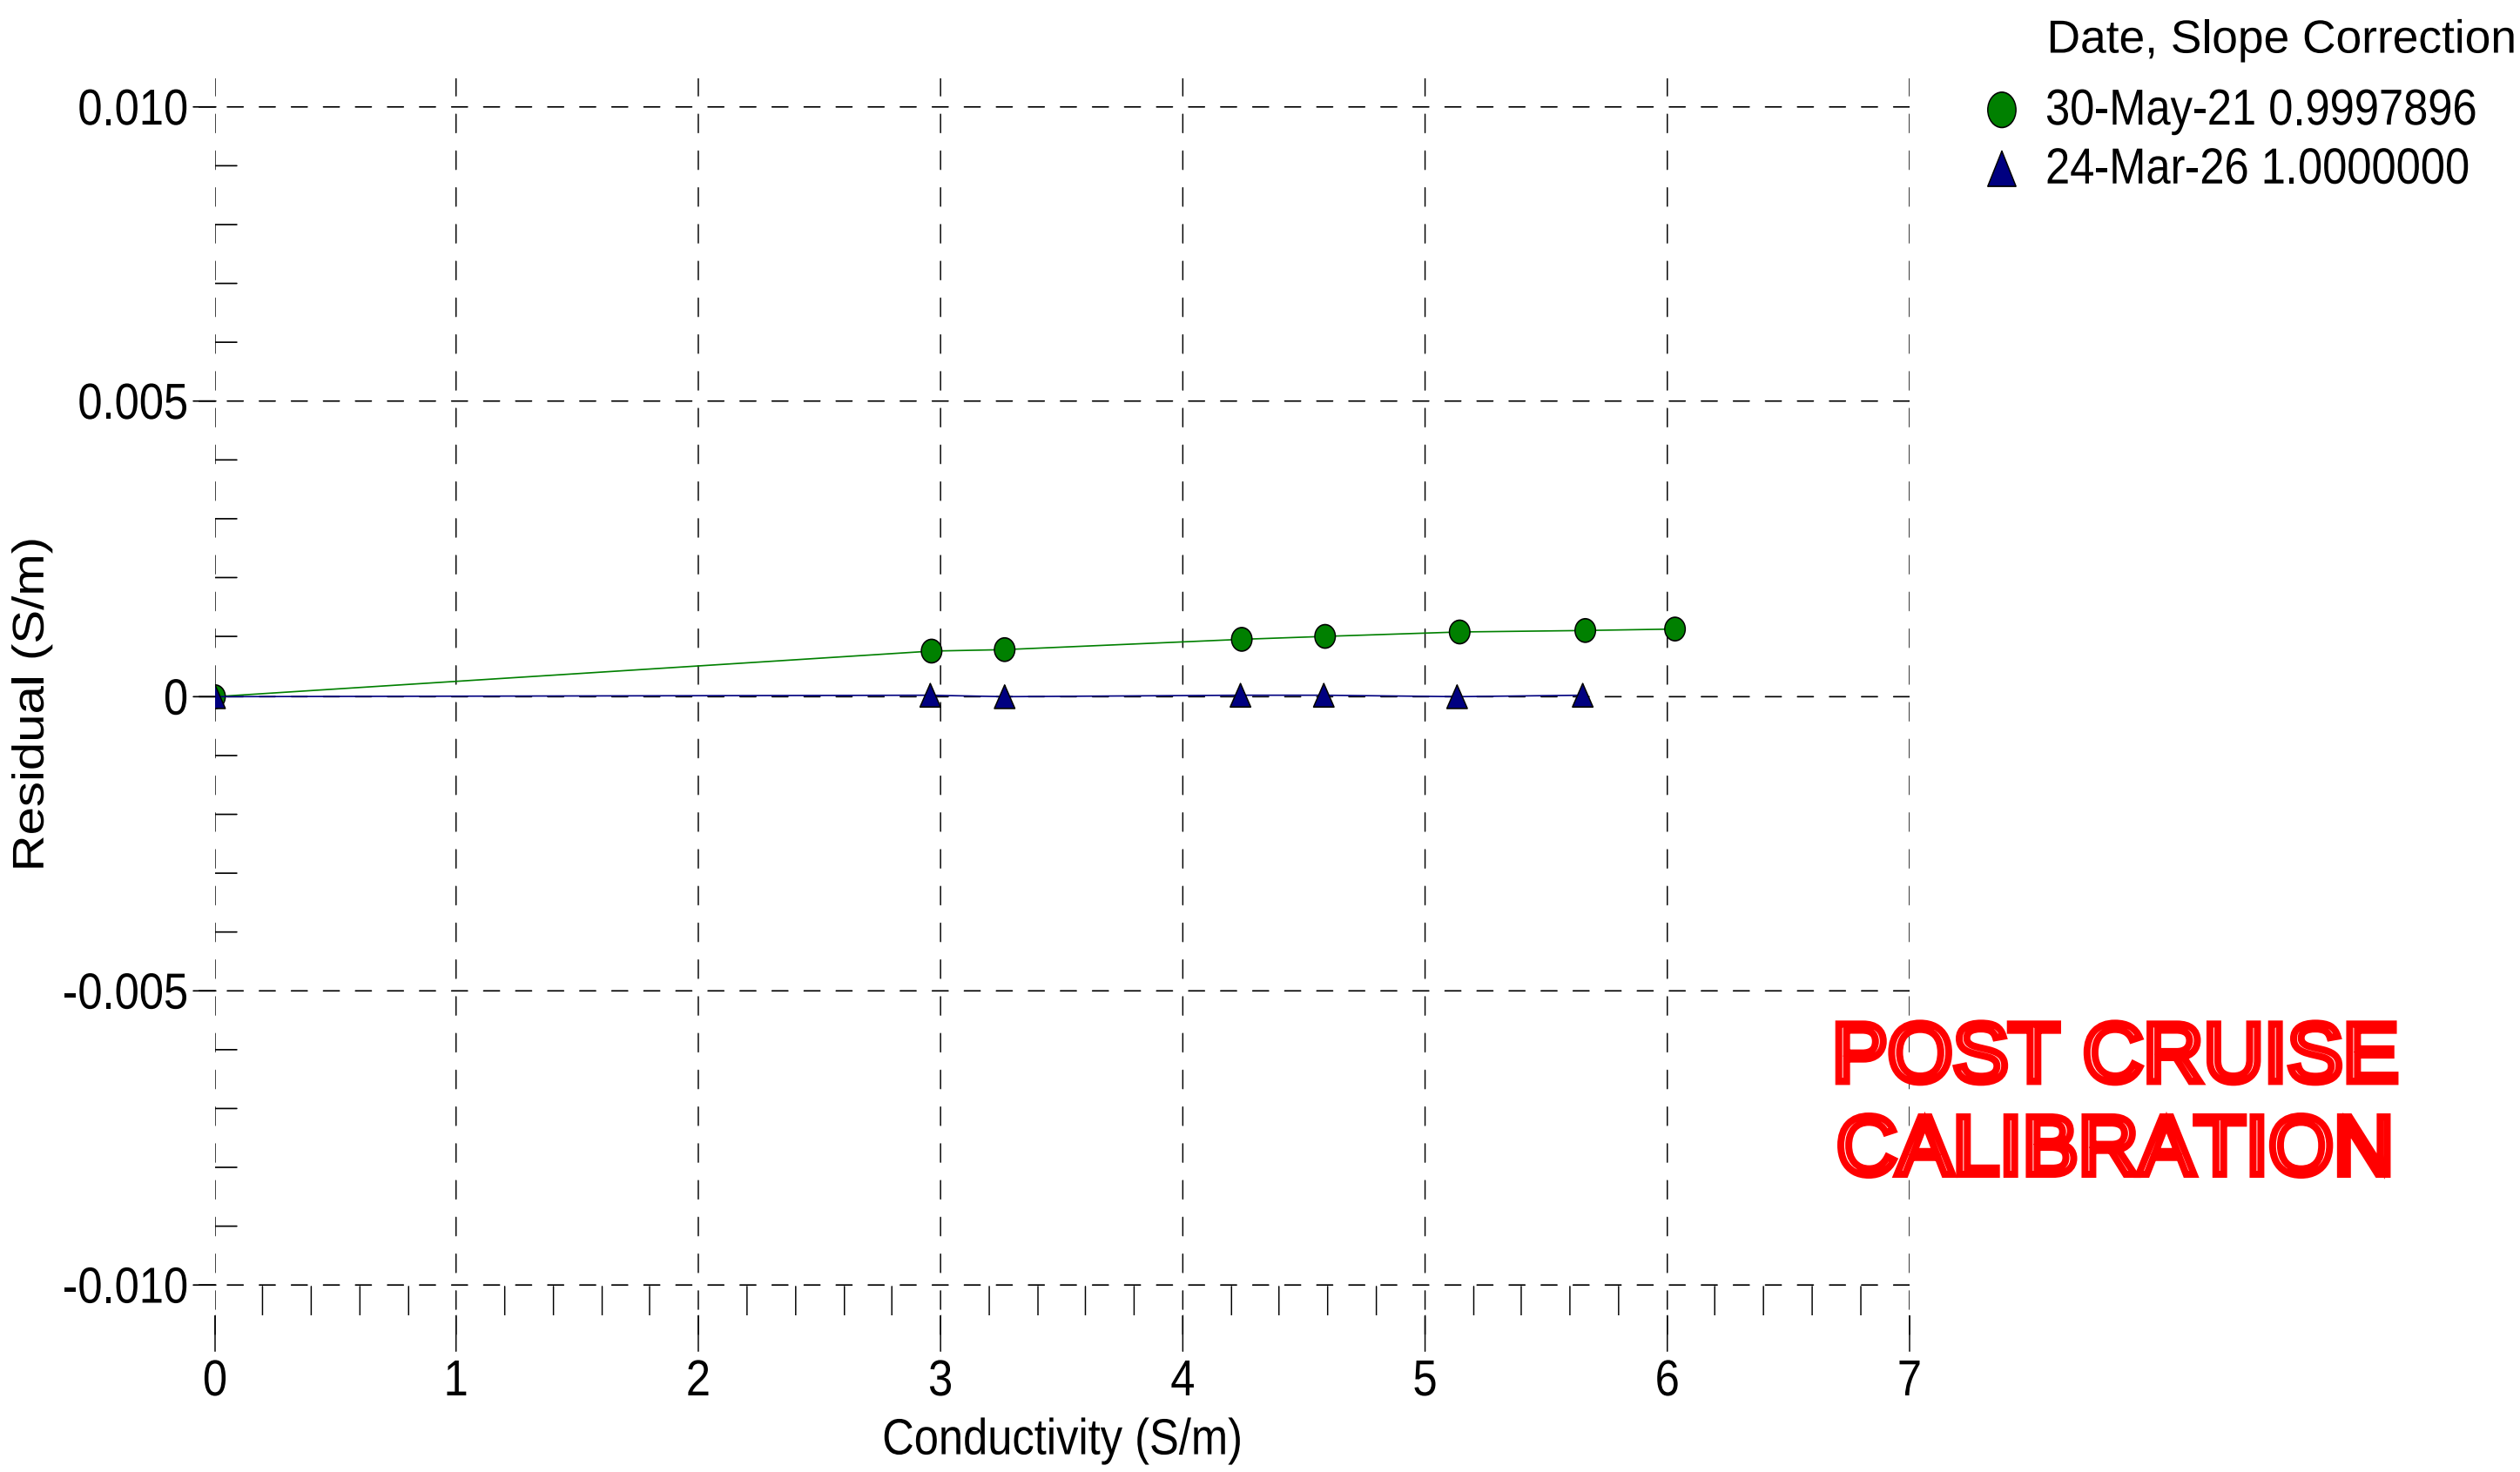

POST CRUISE CALIBRATION