



Sea-Bird Scientific
13431 NE 20th Street
Bellevue, WA 98005
USA

+1 425-643-9866
seabird@seabird.com
www.seabird.com

SENSOR SERIAL NUMBER: 0027
CALIBRATION DATE: 05-Mar-26

Prawler CTD PRESSURE CALIBRATION DATA
870 psia S/N 4434657

COEFFICIENTS:

PA0 =	3.813886e-01	PTCA0 =	5.236193e+05
PA1 =	2.717528e-03	PTCA1 =	1.048327e+01
PA2 =	6.606240e-11	PTCA2 =	-1.826065e-01
PTEMPA0 =	2.202329e+02	PTCB0 =	2.488900e+01
PTEMPA1 =	-6.096528e-02	PTCB1 =	1.000000e-03
PTEMPA2 =	-3.507878e-06	PTCB2 =	0.000000e+00

PRESSURE SPAN CALIBRATION

THERMAL CORRECTION

PRESSURE (PSIA)	INSTRUMENT OUTPUT (counts)	THERMISTOR OUTPUT (volts)	COMPUTED PRESSURE (PSIA)	RESIDUAL (%FSR)	TEMP (°C)	THERMISTOR OUTPUT (volts)	INSTRUMENT OUTPUT (counts)
14.66	529038.0	2794.0	14.71	0.01	32.50	2670	529396.20
179.86	589741.0	2790.0	179.80	-0.01	29.00	2712	529400.60
359.94	655764.0	2789.0	359.92	-0.00	24.00	2776	529397.60
539.93	721549.0	2789.0	539.95	0.00	18.50	2843	529380.20
719.97	787121.0	2785.0	719.97	0.00	15.00	2887	529364.60
869.98	841587.0	2787.0	869.93	-0.00	4.50	3016	529293.00
719.93	787121.0	2786.0	719.97	0.00	1.00	3058	529260.00
539.92	721551.0	2788.0	539.96	0.00	TEMPERATURE (°C)		SPAN
359.94	655774.0	2788.0	359.94	0.00			
179.93	589780.0	2791.0	179.91	-0.00			
14.66	529024.0	2790.0	14.67	0.00			
					-5.00		24.88
					35.00		24.92

y = thermistor output (counts)

$$t = PTEMPA0 + PTEMPA1 * y + PTEMPA2 * y^2$$

$$x = \text{instrument output} - PTCA0 - PTCA1 * t - PTCA2 * t^2$$


$$n = x * PTCB0 / (PTCB0 + PTCB1 * t + PTCB2 * t^2)$$

$$\text{pressure (PSIA)} = PA0 + PA1 * n + PA2 * n^2$$

$$\text{Residual (\%FSR)} = (\text{computed pressure} - \text{true pressure}) * 100 / \text{Full Scale Range}$$

Date, Offset (%FSR)

● 20-Feb-19 0.06
▲ 05-Mar-26 0.00

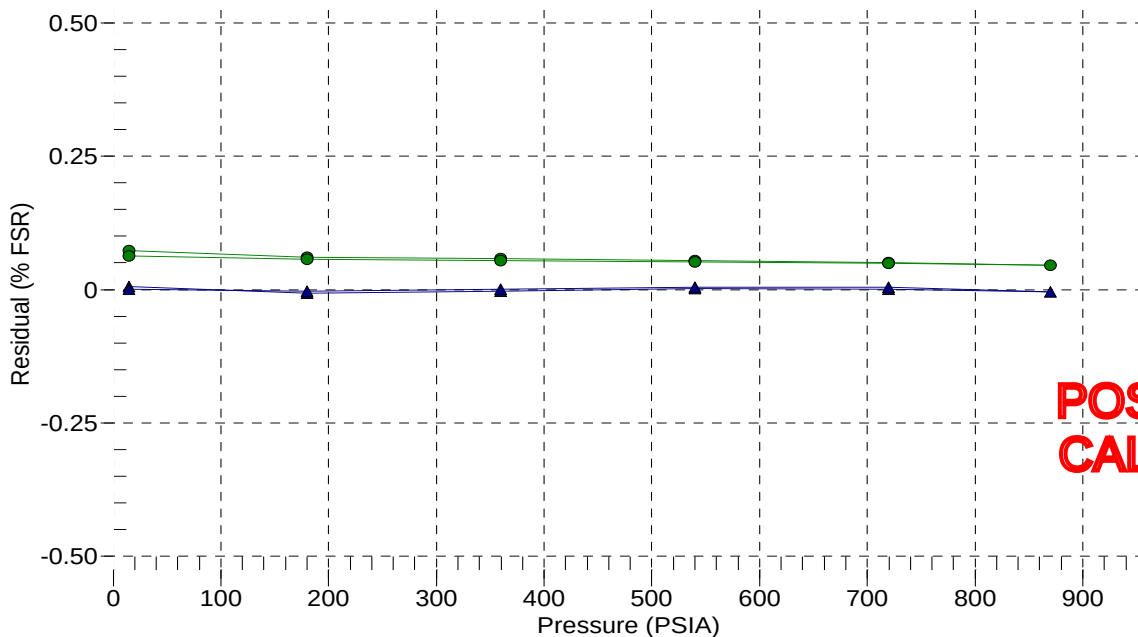

**POST CRUISE
CALIBRATION**