



Sea-Bird Scientific  
13431 NE 20<sup>th</sup> Street  
Bellevue, WA 98005  
USA

+1 425-643-9866  
seabird@seabird.com  
www.seabird.com

SENSOR SERIAL NUMBER: 0045  
CALIBRATION DATE: 05-Mar-26

Prawler CTD PRESSURE CALIBRATION DATA  
870 psia S/N 11573953

COEFFICIENTS:

PA0 = 8.279624e-02  
PA1 = 2.672880e-03  
PA2 = 1.582457e-11  
PTEMPA0 = -8.130079e+01  
PTEMPA1 = 4.617431e-02  
PTEMPA2 = -9.246320e-09

PTCA0 = 5.244559e+05  
PTCA1 = 2.090219e+00  
PTCA2 = -3.163042e-02  
PTCB0 = 2.533734e+01  
PTCB1 = 2.225000e-03  
PTCB2 = 0.000000e+00

PRESSURE SPAN CALIBRATION

THERMAL CORRECTION

| PRESSURE<br>(PSIA) | INSTRUMENT<br>OUTPUT (counts) | THERMISTOR<br>OUTPUT (volts) | COMPUTED<br>PRESSURE (PSIA) | RESIDUAL<br>(%FSR) | TEMP<br>(°C)     | THERMISTOR<br>OUTPUT (volts) | INSTRUMENT<br>OUTPUT (counts) |
|--------------------|-------------------------------|------------------------------|-----------------------------|--------------------|------------------|------------------------------|-------------------------------|
| 14.66              | 529964.0                      | 2253.0                       | 14.69                       | 0.00               | 32.50            | 2466                         | 530190.60                     |
| 179.86             | 591842.0                      | 2253.0                       | 179.83                      | -0.00              | 29.00            | 2390                         | 530193.00                     |
| 359.94             | 659256.0                      | 2253.0                       | 359.87                      | -0.01              | 24.00            | 2282                         | 530192.00                     |
| 539.93             | 726621.0                      | 2253.0                       | 539.93                      | -0.00              | 18.50            | 2162                         | 530185.40                     |
| 719.97             | 793920.0                      | 2254.0                       | 719.95                      | -0.00              | 15.00            | 2086                         | 530180.40                     |
| 869.98             | 849943.0                      | 2254.0                       | 869.92                      | -0.01              | 4.50             | 1859                         | 530165.60                     |
| 719.93             | 793936.0                      | 2254.0                       | 720.00                      | 0.01               | 1.00             | 1783                         | 530161.00                     |
| 539.92             | 726644.0                      | 2253.0                       | 539.99                      | 0.01               |                  |                              |                               |
| 359.94             | 659281.0                      | 2253.0                       | 359.94                      | 0.00               | TEMPERATURE (°C) |                              | SPAN                          |
| 179.93             | 591870.0                      | 2253.0                       | 179.90                      | -0.00              | -4.20            |                              | 25.33                         |
| 14.66              | 529957.0                      | 2253.0                       | 14.67                       | 0.00               | 35.80            |                              | 25.42                         |

y = thermistor output (counts)

t = PTEMPA0 + PTEMPA1 \* y + PTEMPA2 \* y<sup>2</sup>

x = instrument output - PTCA0 - PTCA1 \* t - PTCA2 \* t<sup>2</sup>


n = x \* PTCB0 / (PTCB0 + PTCB1 \* t + PTCB2 \* t<sup>2</sup>)

pressure (PSIA) = PA0 + PA1 \* n + PA2 \* n<sup>2</sup>

Residual (%FSR) = (computed pressure - true pressure) \* 100 / Full Scale Range

Date, Offset (%FSR)

● 27-Apr-23 0.02  
▲ 05-Mar-26 -0.00

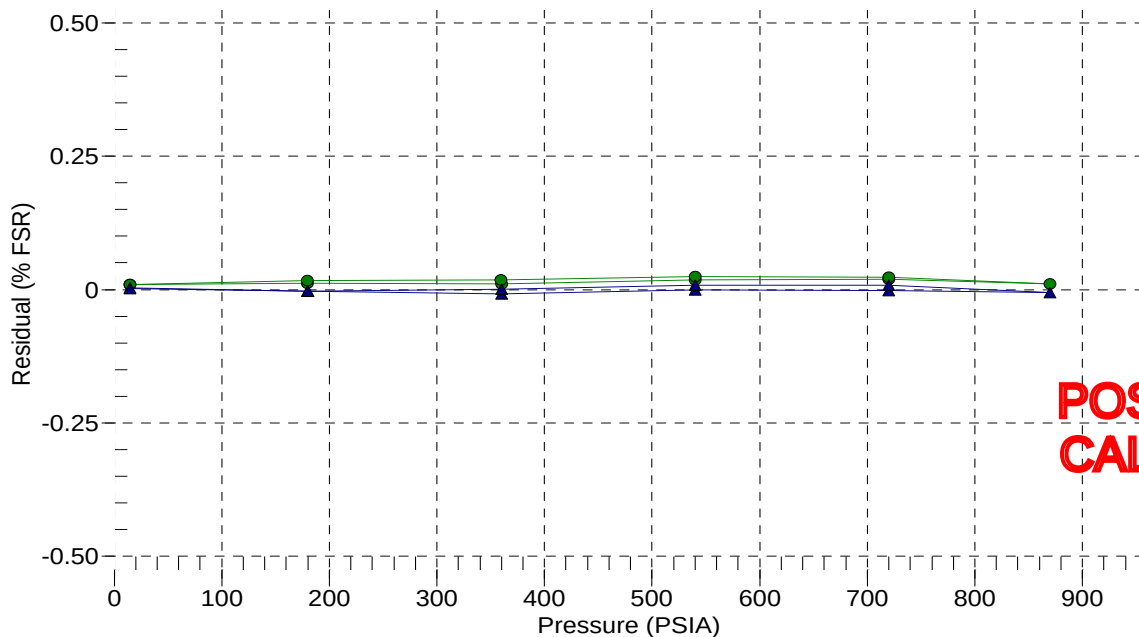

**POST CRUISE  
CALIBRATION**