



Sea-Bird Scientific
13431 NE 20th Street
Bellevue, WA 98005
USA

+1 425-643-9866
seabird@seabird.com
www.seabird.com

SENSOR SERIAL NUMBER: 1624
CALIBRATION DATE: 09-Feb-26

SBE 39 PRESSURE CALIBRATION DATA
508 psia S/N 5503

COEFFICIENTS:

PA0 =	-1.374514e+02	PTCA0 =	-1.012467e+01
PA1 =	1.448945e+00	PTCA1 =	3.403010e-01
PA2 =	7.538679e-07	PTCA2 =	-1.023848e-02
PTHA0 =	-8.210133e+01	PTCB0 =	2.509938e+01
PTHA1 =	4.821853e-02	PTCB1 =	2.763819e-04
PTHA2 =	-4.167875e-07	PTCB2 =	0.000000e+00

PRESSURE SPAN CALIBRATION

THERMAL CORRECTION

PRESSURE (PSIA)	INSTRUMENT OUTPUT (counts)	THERMISTOR OUTPUT (counts)	COMPUTED PRESSURE (PSIA)	RESIDUAL (%FSR)	TEMP (°C)	THERMISTOR OUTPUT (counts)	INSTRUMENT OUTPUT (counts)
14.64	-0.0	22.5	14.66	0.00	-1.50	1696.40	576.30
104.89	62.2	22.8	104.84	-0.01	1.00	1749.90	577.18
204.89	131.1	22.6	204.88	-0.00	4.50	1824.80	578.18
304.89	200.1	22.6	304.88	-0.00	8.00	1900.00	578.86
404.89	269.0	22.5	404.89	-0.00	11.50	1975.00	579.44
504.87	337.9	22.5	504.86	-0.00	15.00	2049.80	579.62
404.89	269.0	22.6	404.90	0.00	18.50	2125.40	579.97
304.90	200.1	22.7	304.91	0.00	22.00	2200.80	579.30
204.90	131.2	22.6	204.92	0.00	25.50	2276.40	578.81
104.90	62.2	22.6	104.92	0.00	29.00	2352.00	577.67
14.65	-0.0	22.6	14.64	-0.00	32.50	2427.60	577.42

TEMPERATURE (°C)	SPAN
-5.00	25.10
34.80	25.11

y = thermistor output (counts)

t = PTHA0 + PTHA1 * y + PTHA2 * y²

x = instrument output - PTCA0 - PTCA1 * t - PTCA2 * t²


n = x * PTCB0 / (PTCB0 + PTCB1 * t + PTCB2 * t²)

pressure (PSIA) = PA0 + PA1 * n + PA2 * n²

Residual (%FSR) = (computed pressure - true pressure) * 100 / Full Scale Range

Date, Offset (%FSR)

● 06-Oct-16 2735.22
▲ 09-Feb-26 -0.00

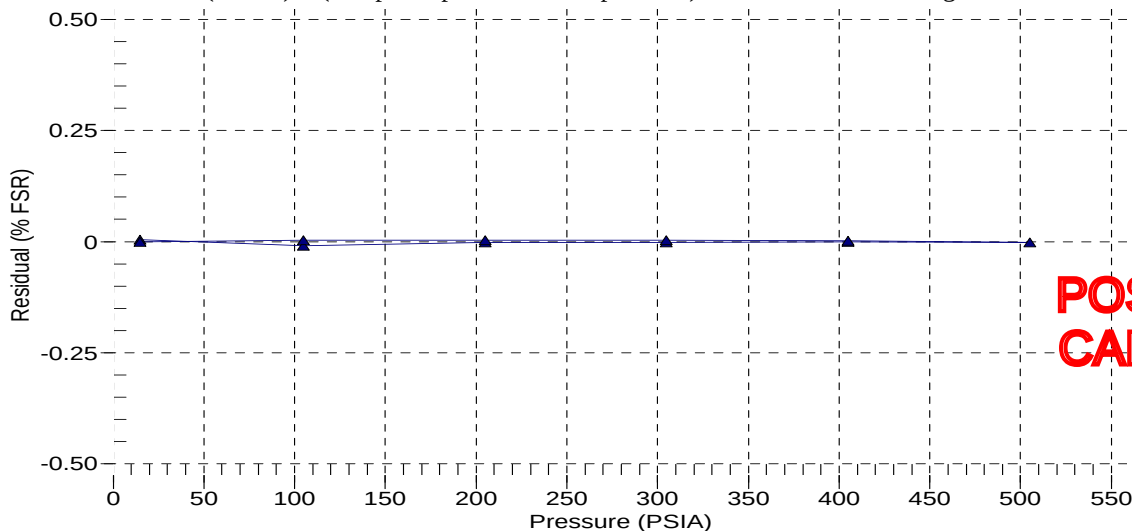

**POST CRUISE
CALIBRATION**