

ECG Signal - Minute 1 (0-30s)

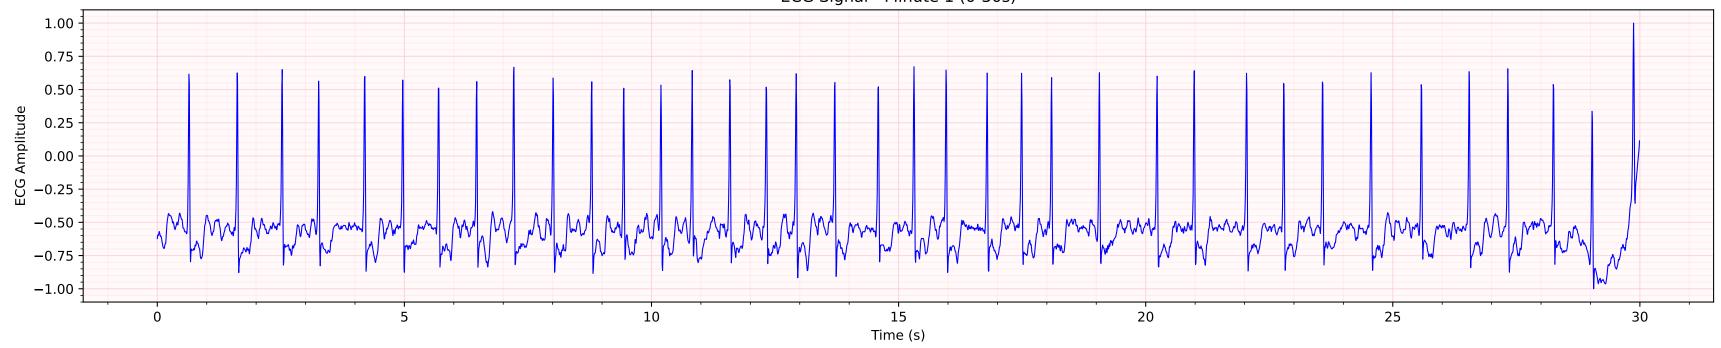

ECG Signal - Minute 1 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 · -0.75-1.0030 35 40 45 50 55

ECG Signal - Minute 2 (0-30s)

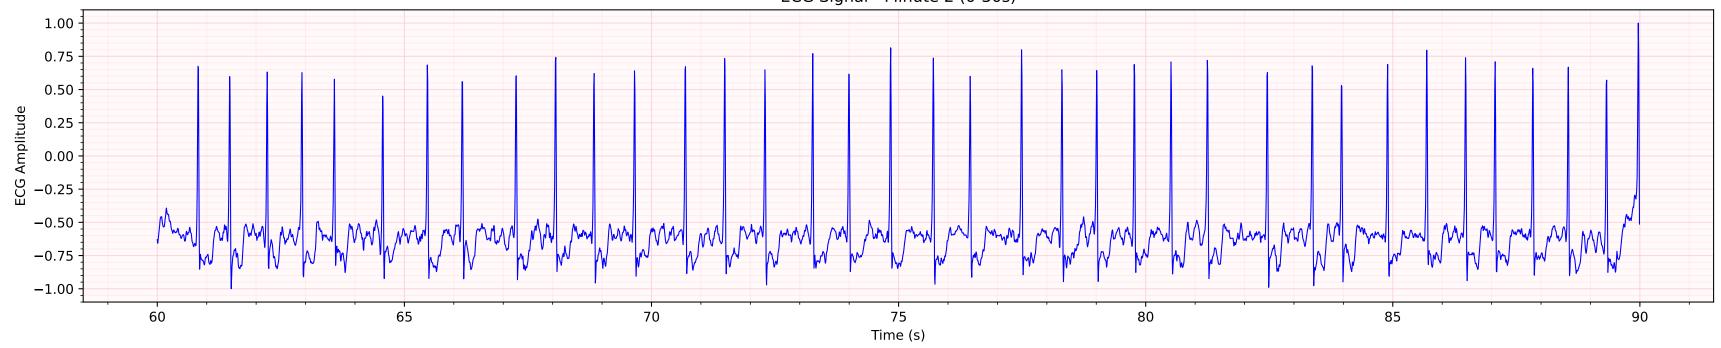

ECG Signal - Minute 2 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 --0.75-1.00

105

Time (s)

110

115

120


100

90


ECG Signal - Minute 3 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 My lm, ⊕ –0.25 -0.50 -




ECG Signal - Minute 3 (30-60s)

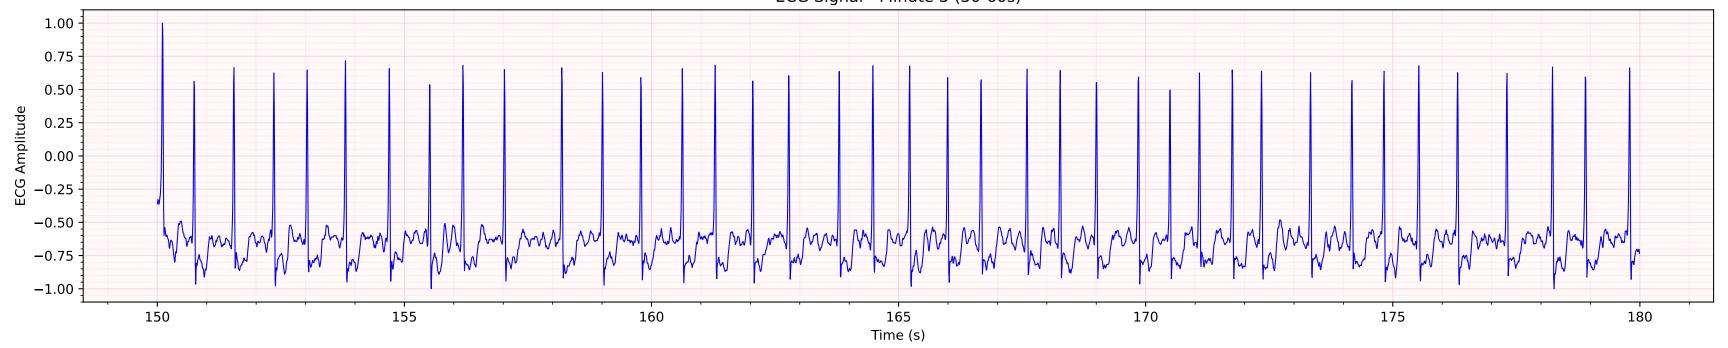


ECG Signal - Minute 4 (0-30s)

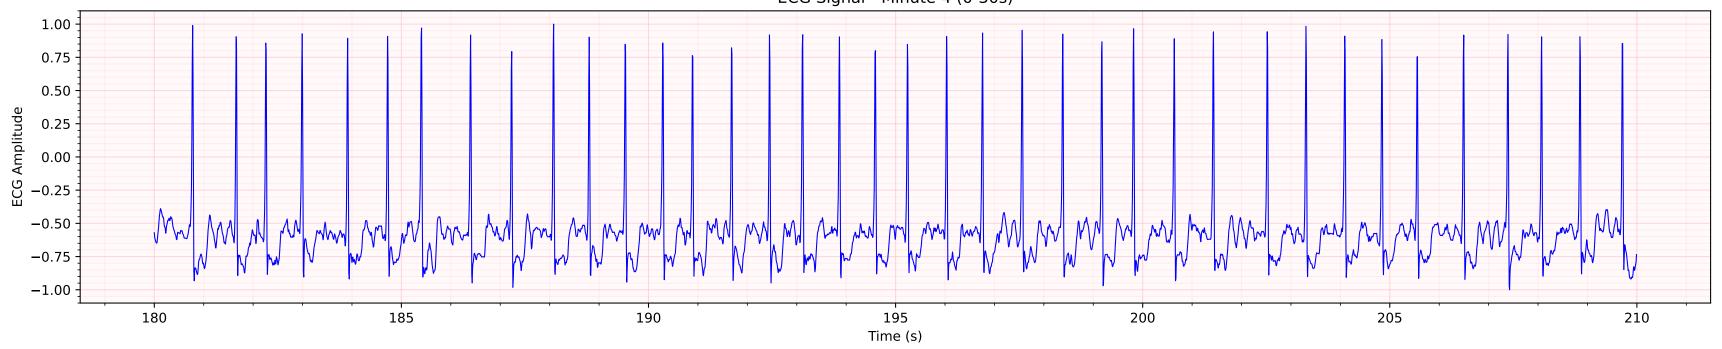


ECG Signal - Minute 4 (30-60s)

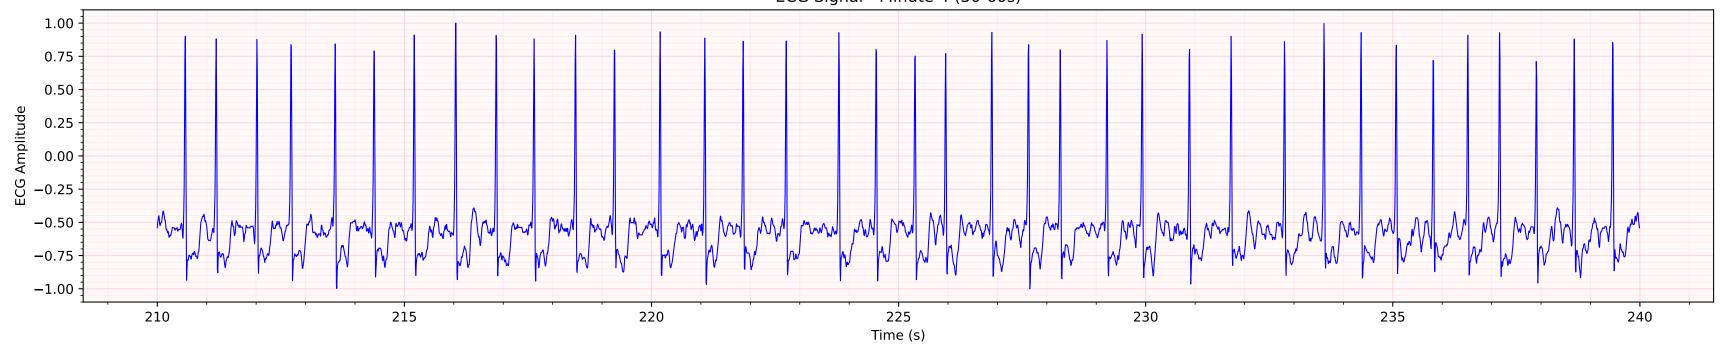


ECG Signal - Minute 5 (0-30s)

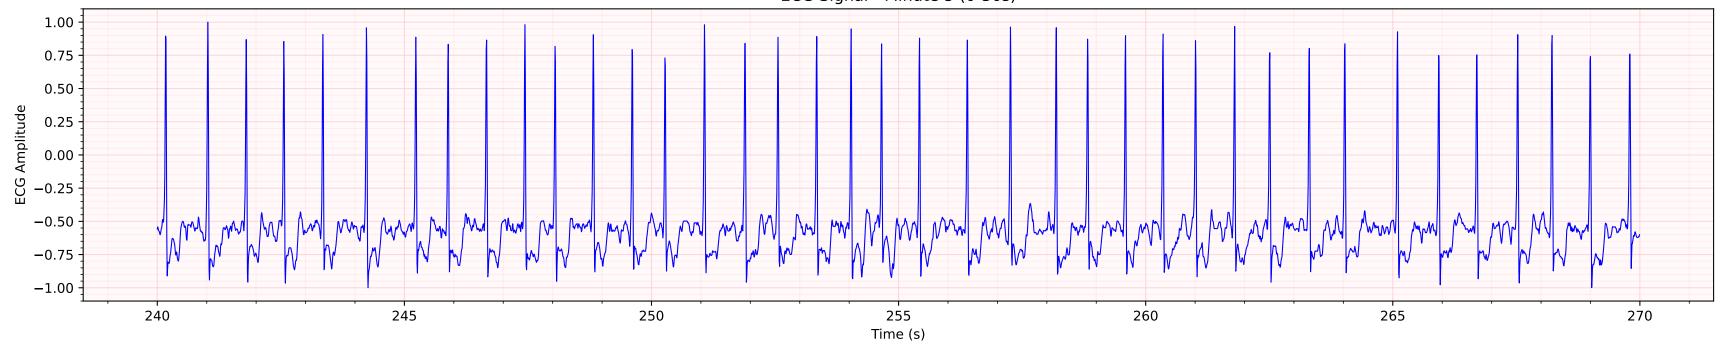


ECG Signal - Minute 5 (30-60s)

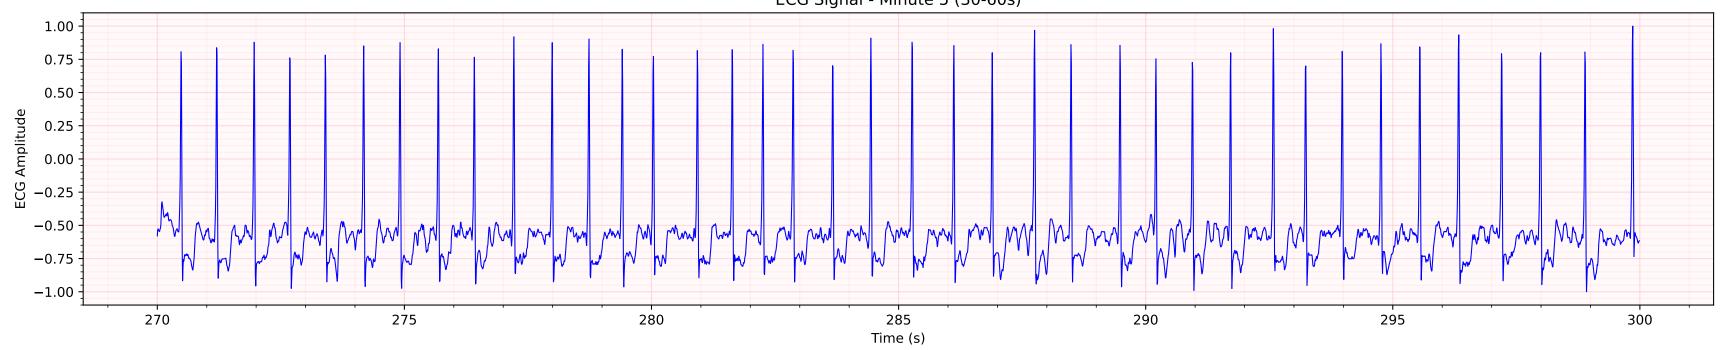


ECG Signal - Minute 6 (0-30s)

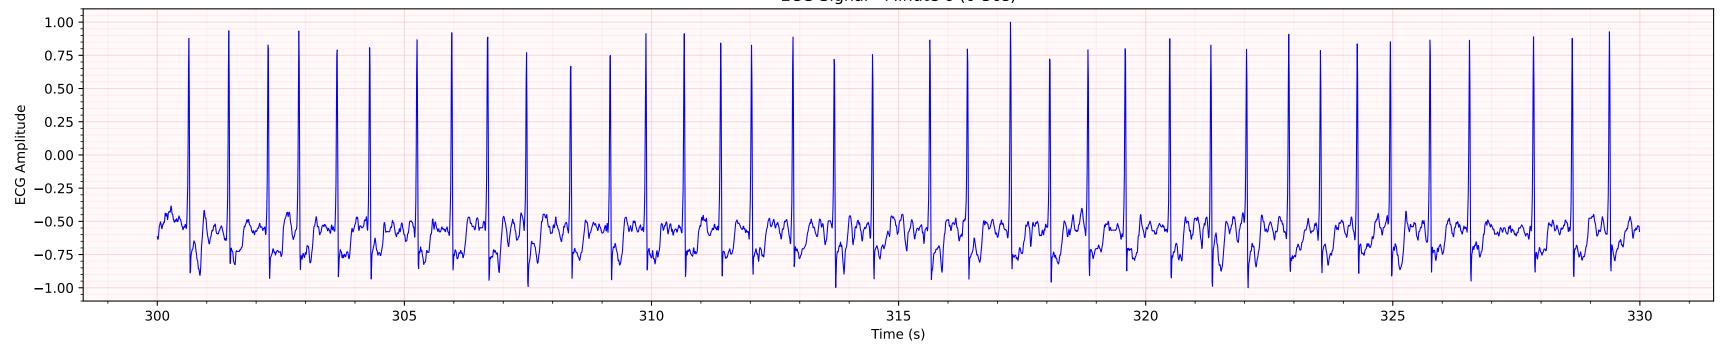


ECG Signal - Minute 6 (30-60s) 1.00 0.75 0.50 Amplitude 0.00

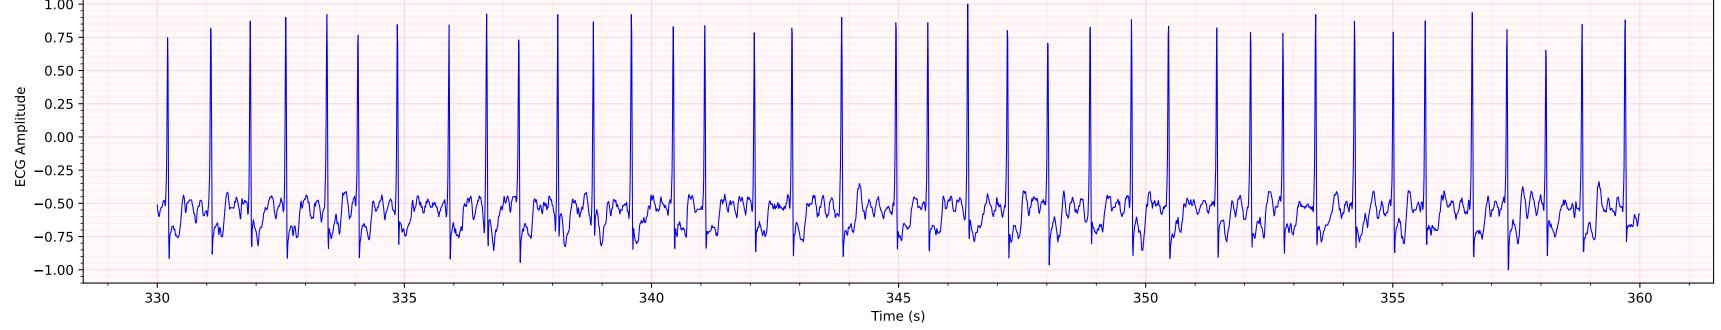


ECG Signal - Minute 7 (0-30s)

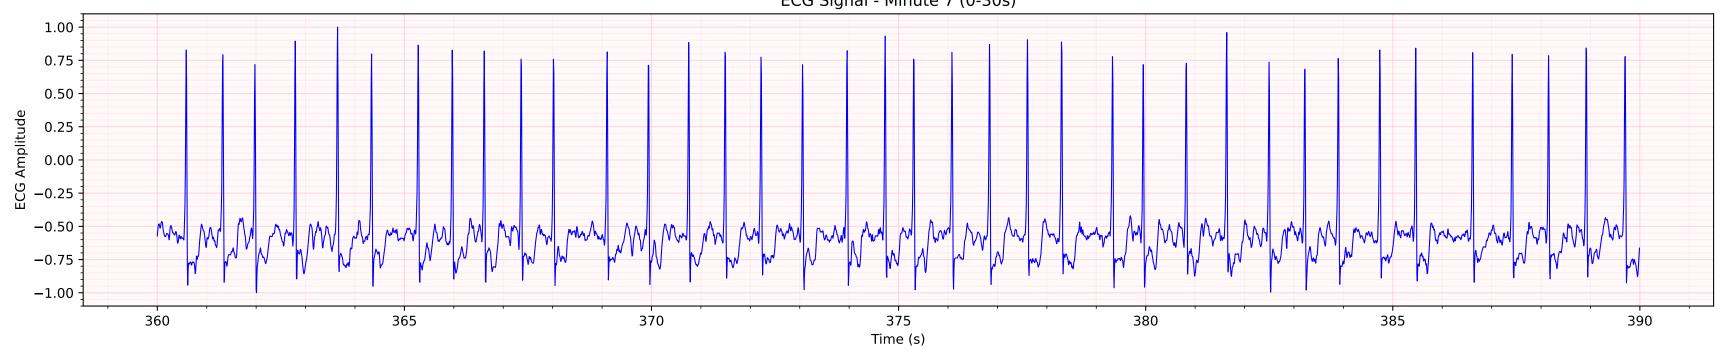


ECG Signal - Minute 7 (30-60s)

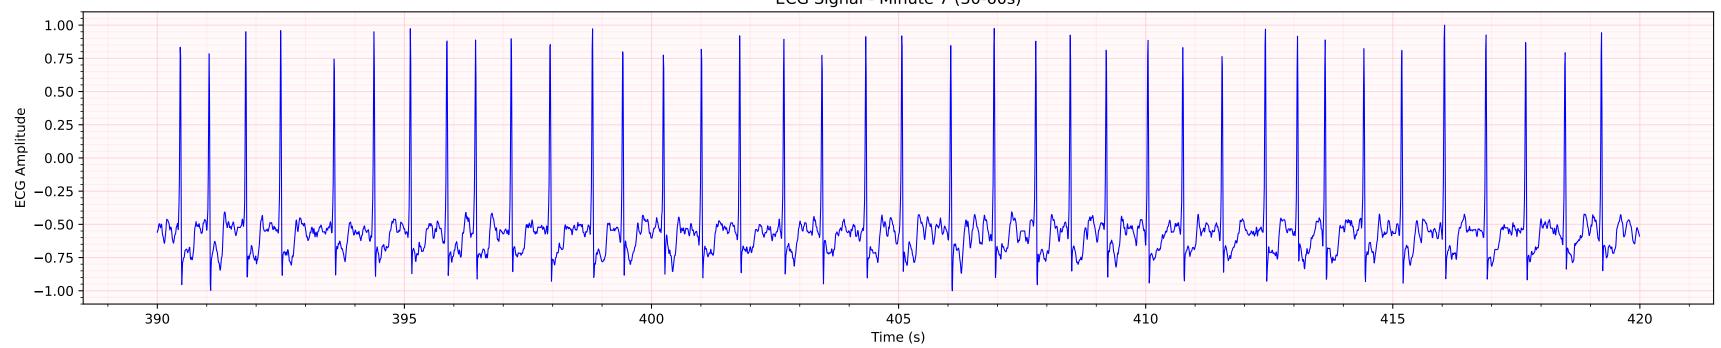


ECG Signal - Minute 8 (0-30s)

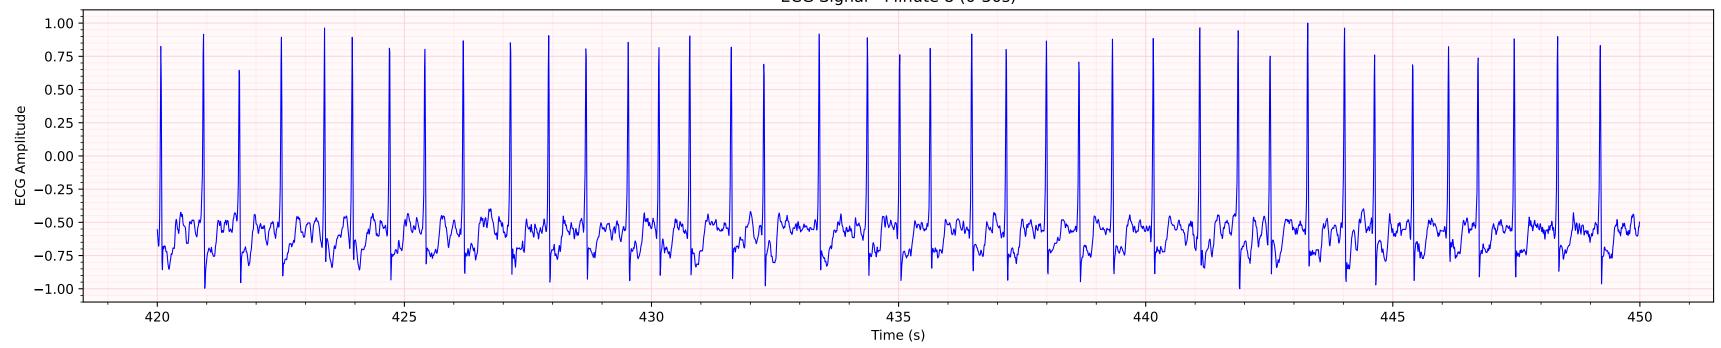


ECG Signal - Minute 8 (30-60s) 1.00 0.75 0.50 Amplitude 0.00

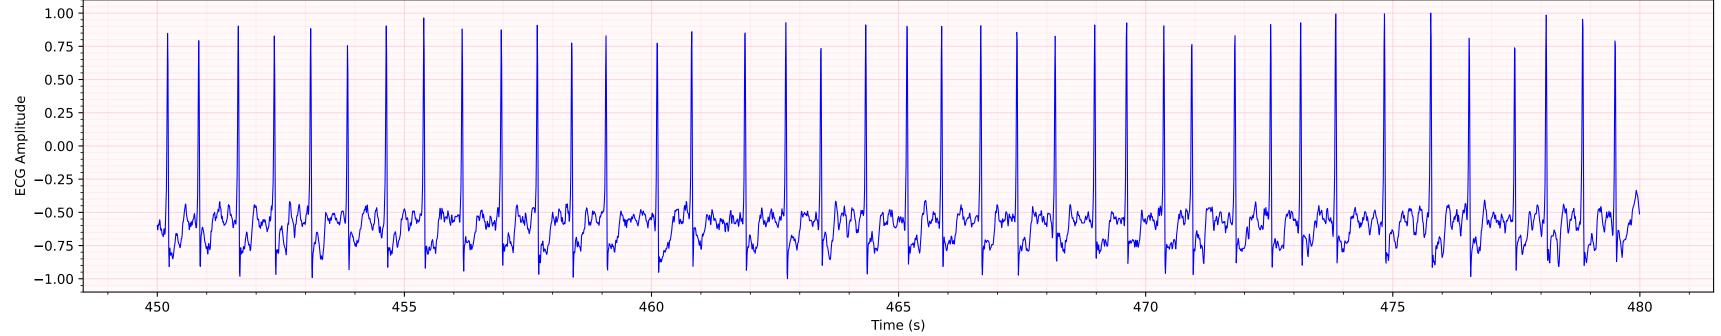


ECG Signal - Minute 9 (0-30s)

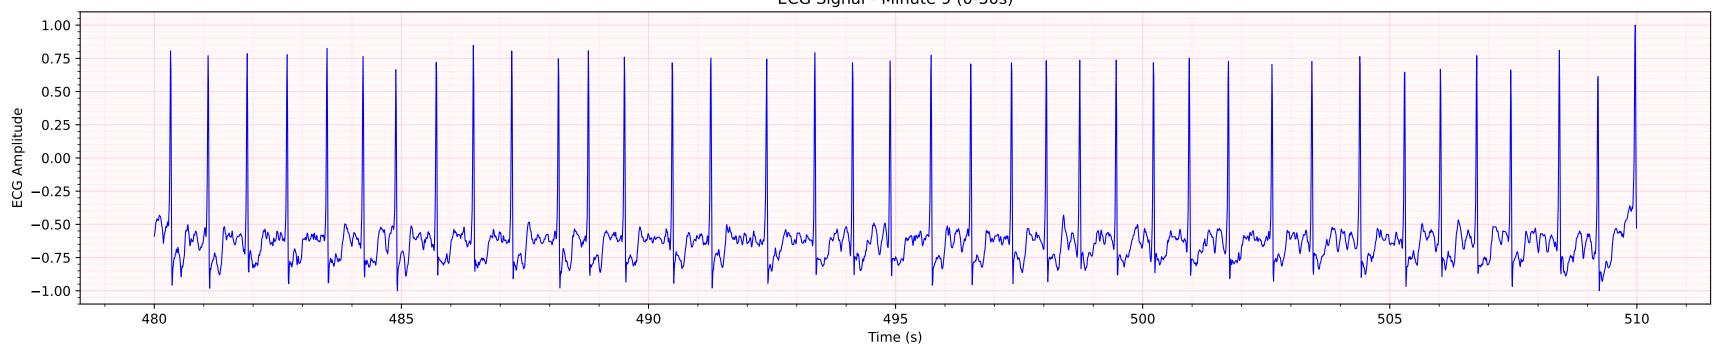

ECG Signal - Minute 9 (30-60s)

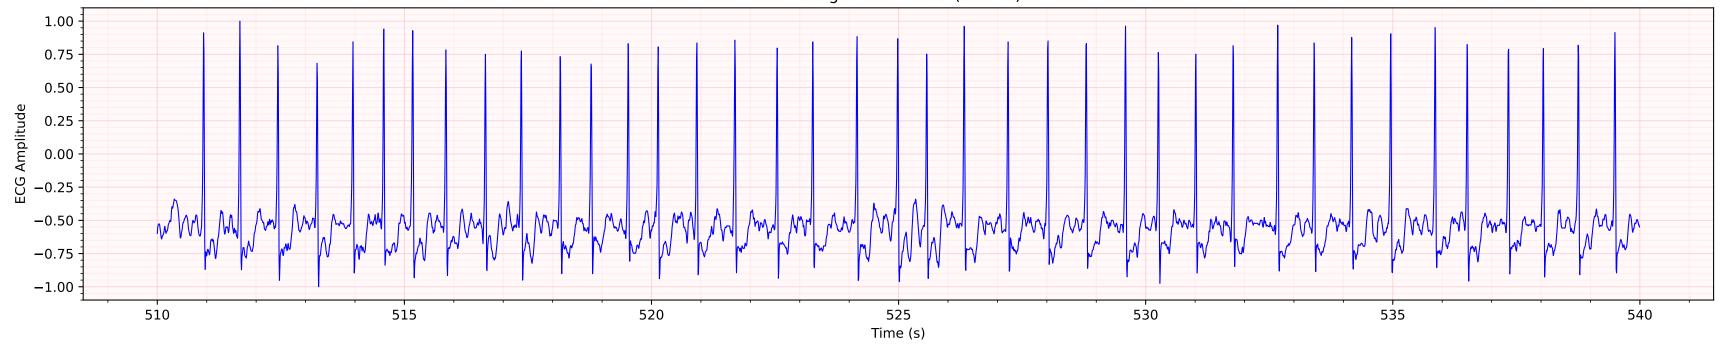


ECG Signal - Minute 10 (0-30s) 1.00 0.75 0.50 Amplitude 0.00

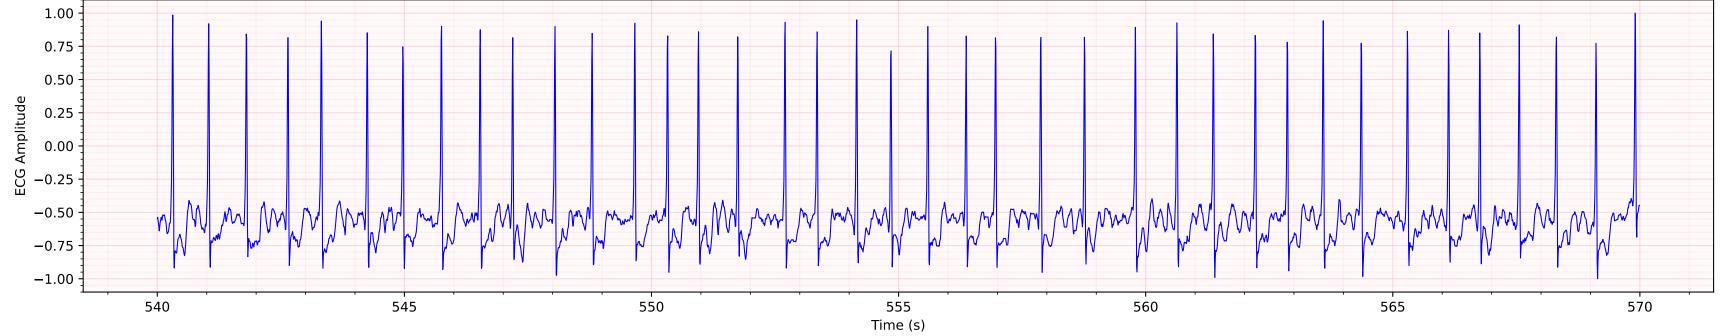

ECG Signal - Minute 10 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50-0.75-1.00570 575 580 585 595 600 590

ECG Signal - Minute 11 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 უ −0.25 -0.50 -0.75-1.00600 605 610 625 630 615 620 Time (s)


ECG Signal - Minute 11 (30-60s)

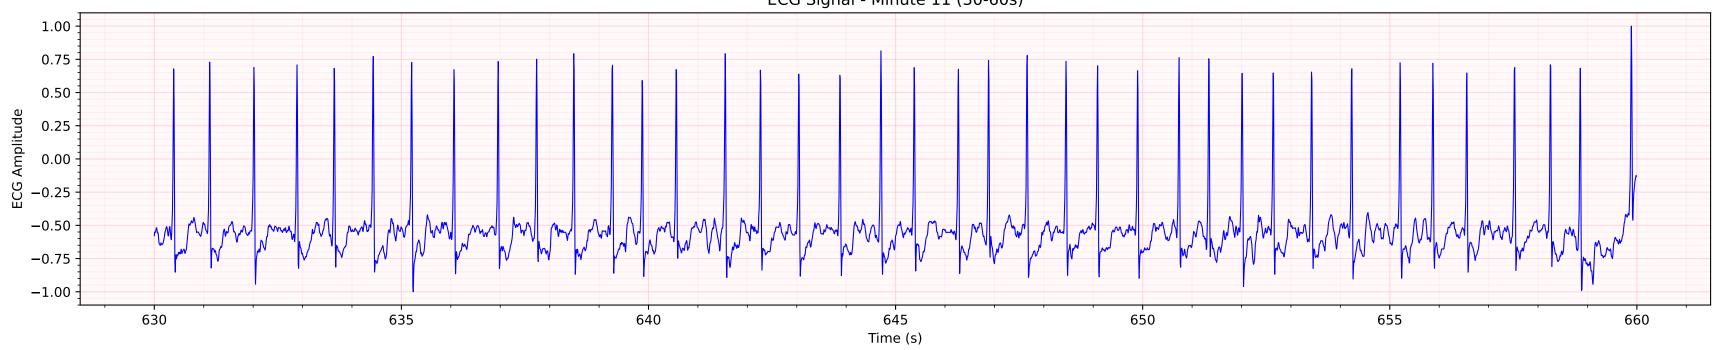

ECG Signal - Minute 12 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 -0.75-1.00660 665 670 685 690 675 680

ECG Signal - Minute 12 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 -0.75-1.00690 695 720 705 710 715

ECG Signal - Minute 13 (0-30s)

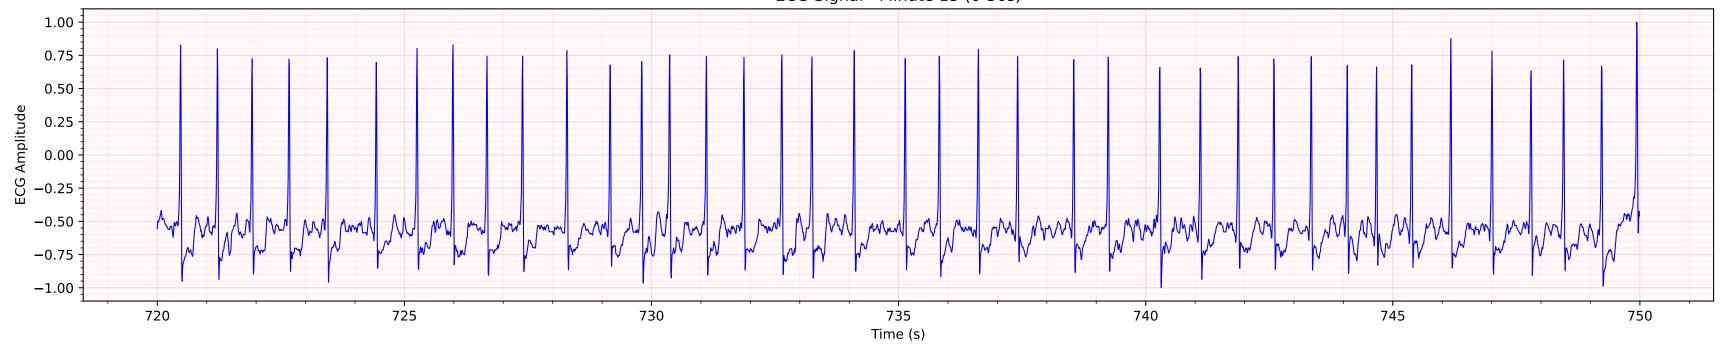

ECG Signal - Minute 13 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ **–**0.25 -0.50 · -0.75-1.00

765

Time (s)

775


770

780


760

750


ECG Signal - Minute 14 (0-30s)

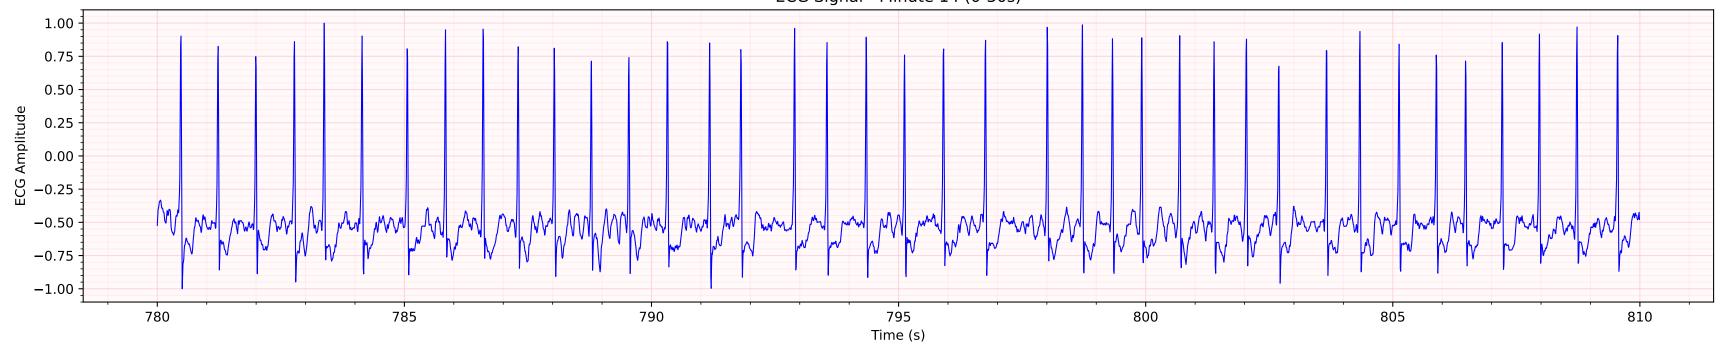


ECG Signal - Minute 14 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 ·

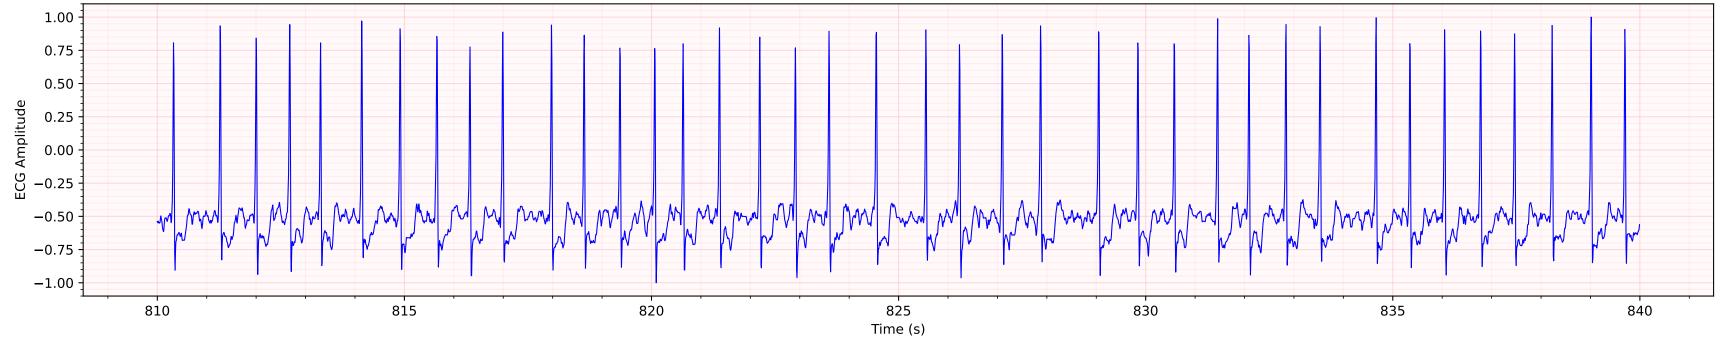


ECG Signal - Minute 15 (0-30s)

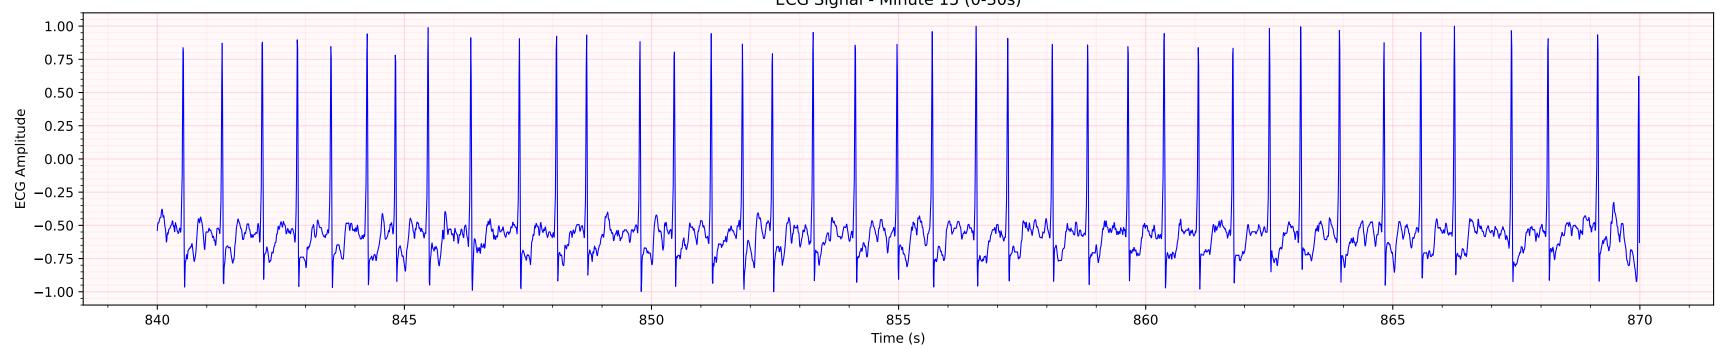

ECG Signal - Minute 15 (30-60s)

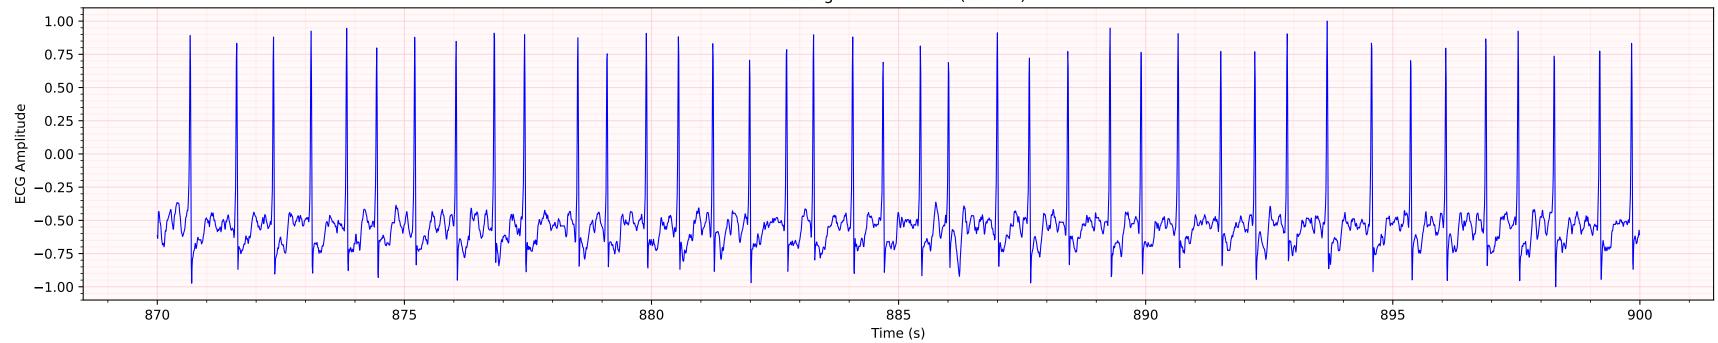

ECG Signal - Minute 16 (0-30s)

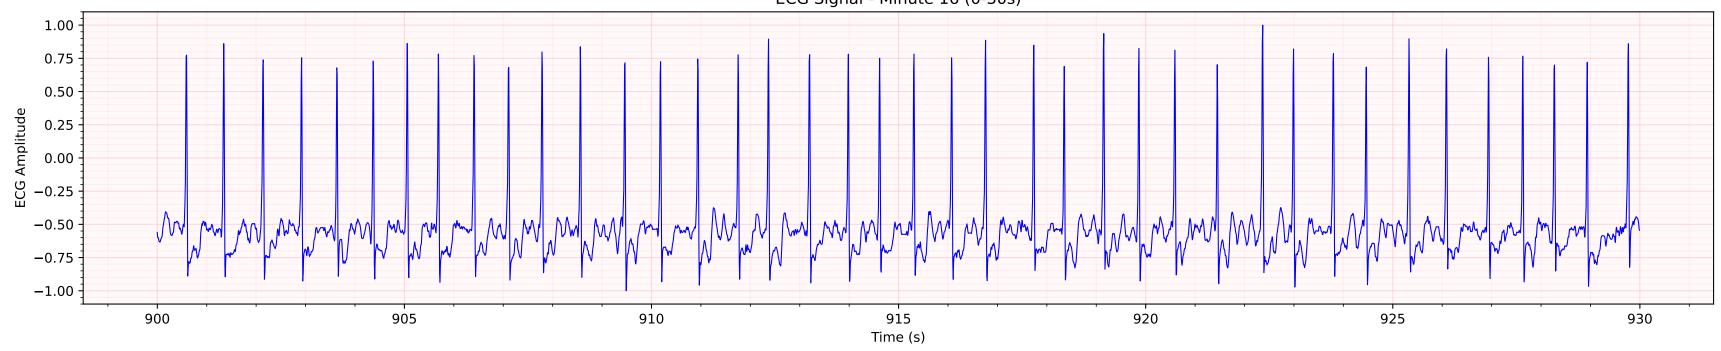

ECG Signal - Minute 16 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 · -0.75-1.00 ·

945

Time (s)

950

955

960

940

930

ECG Signal - Minute 17 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 <u>9</u> –0.25 -0.50 · -0.75

980

985


990

970


-1.00

960


ECG Signal - Minute 17 (30-60s) 1.00 0.75 0.50 Amplitude 0.00

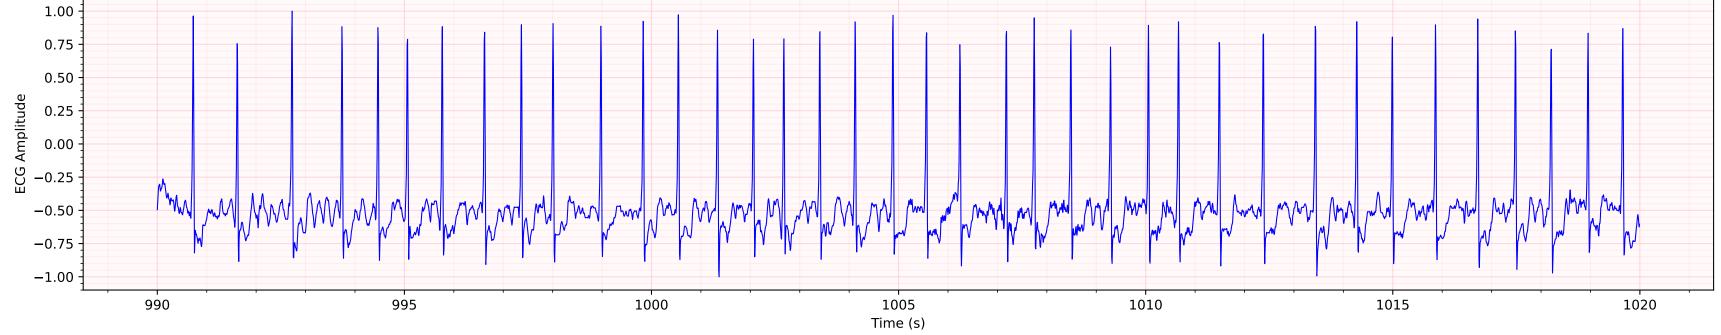


ECG Signal - Minute 18 (0-30s)

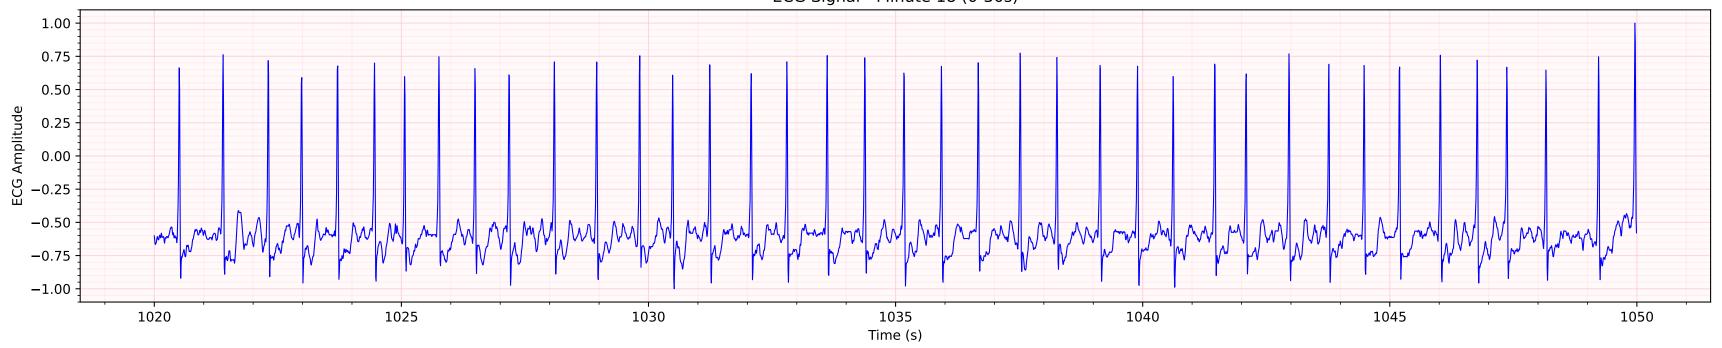


ECG Signal - Minute 18 (30-60s)

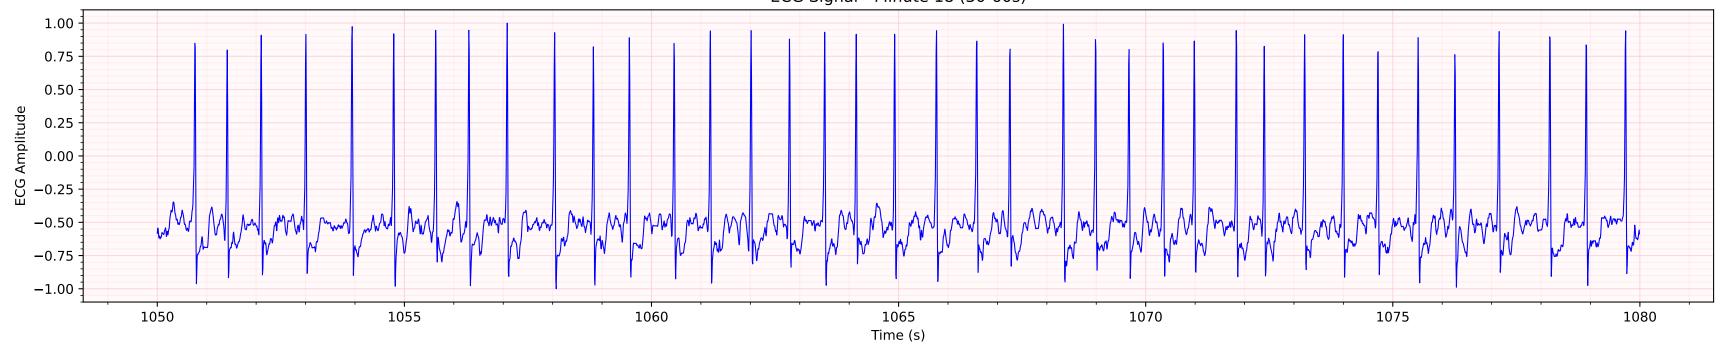


ECG Signal - Minute 19 (0-30s)

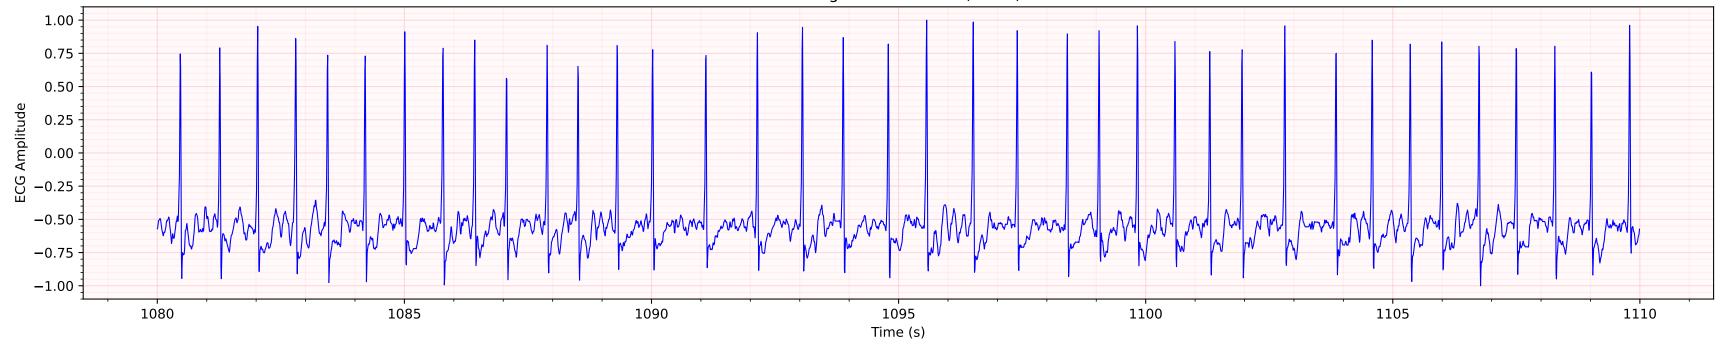

ECG Signal - Minute 19 (30-60s)

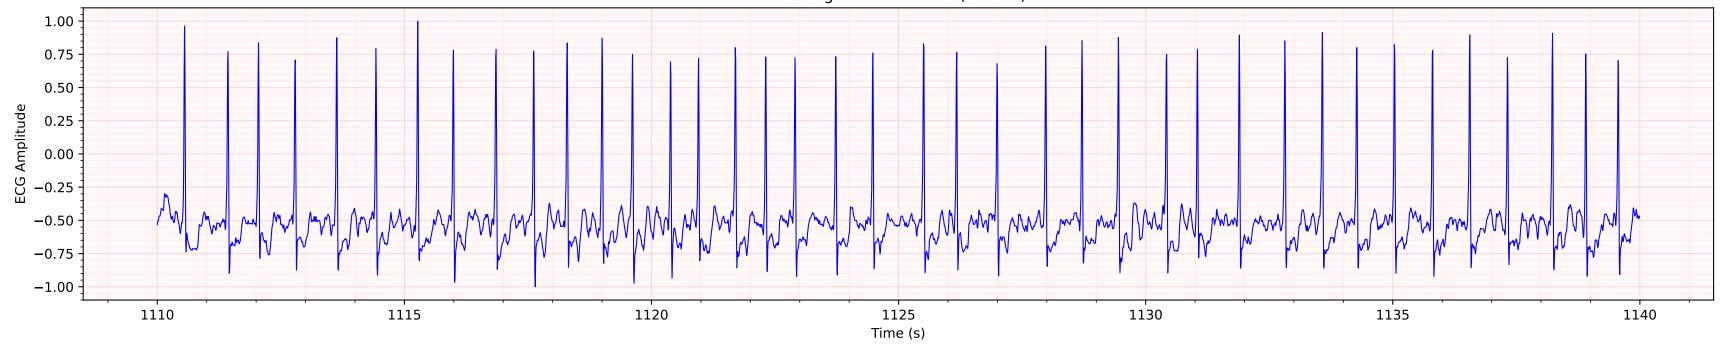

ECG Signal - Minute 20 (0-30s)

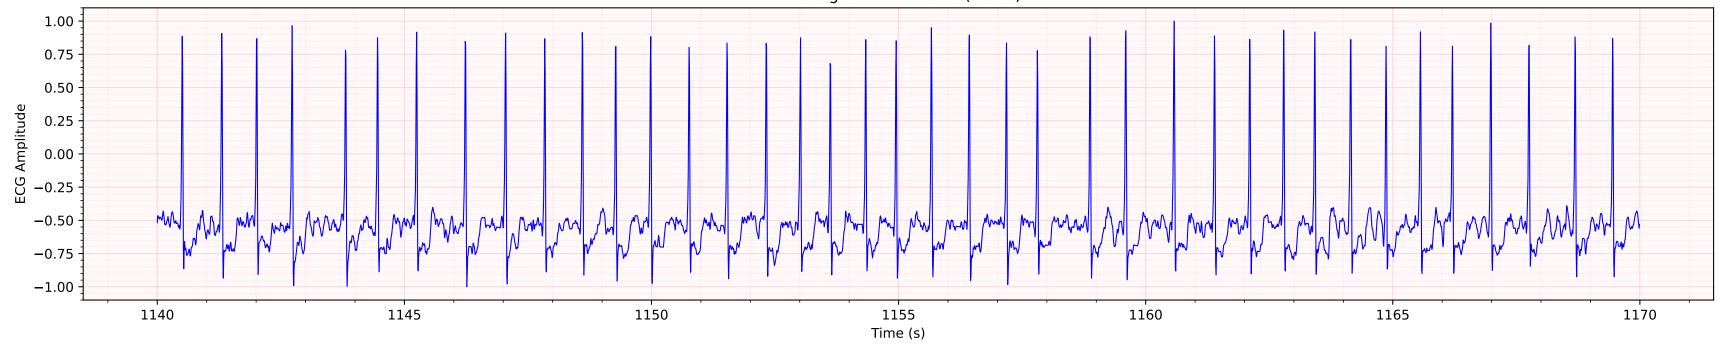

ECG Signal - Minute 20 (30-60s)

