ECG Signal - Minute 1 (0-30s) 1.00 0.75 0.50 ECG Amplitude 0.00 -0.25 --0.50 -0.75 -1.00 ·

ECG Signal - Minute 1 (30-60s) 1.00 0.75 0.50 0.00 - Amplitude ⊕ −0.25 -0.50 --0.75-1.0030 35 40 55 Time (s)

ECG Signal - Minute 2 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 --0.75-1.00


80

85


70

60


ECG Signal - Minute 2 (30-60s) 1.00 0.75 0.50

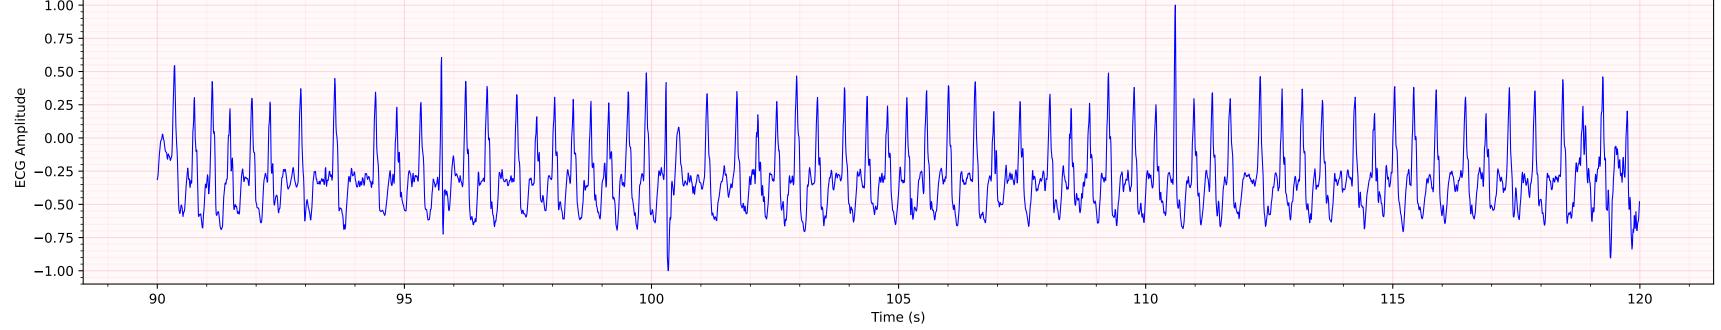


ECG Signal - Minute 3 (0-30s) 1.00 0.75

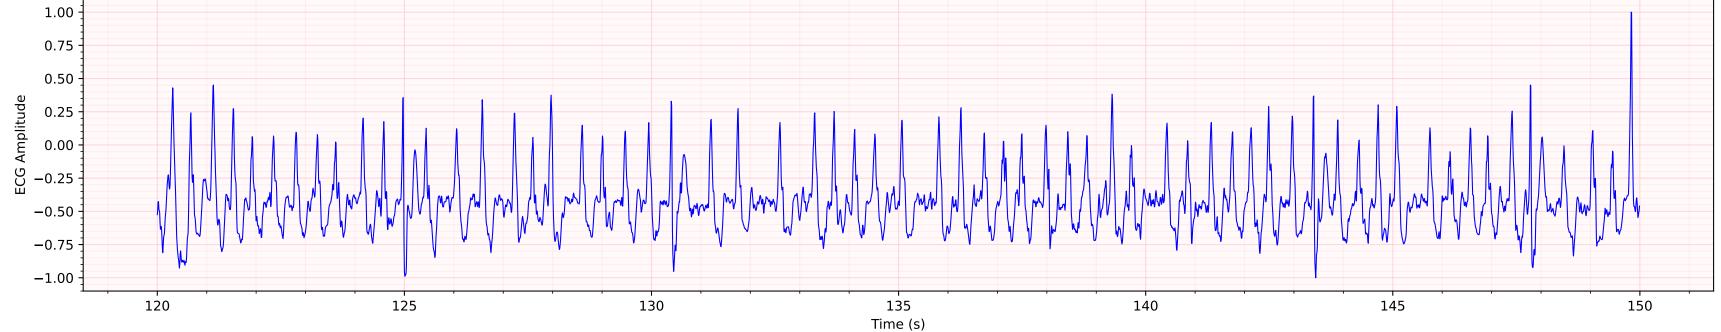


ECG Signal - Minute 3 (30-60s) 1.00 0.75 0.50 Amplitude 0.00

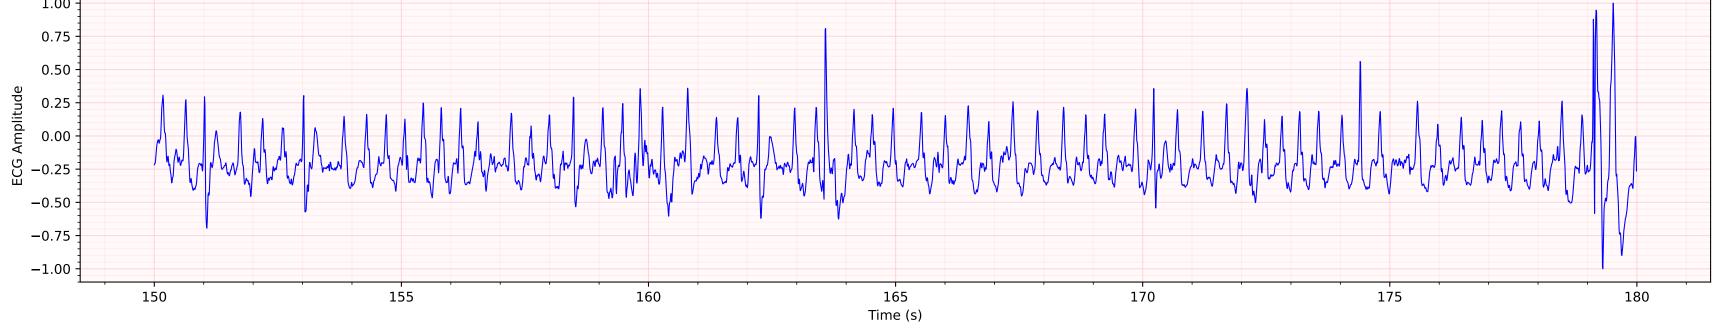


ECG Signal - Minute 4 (0-30s)

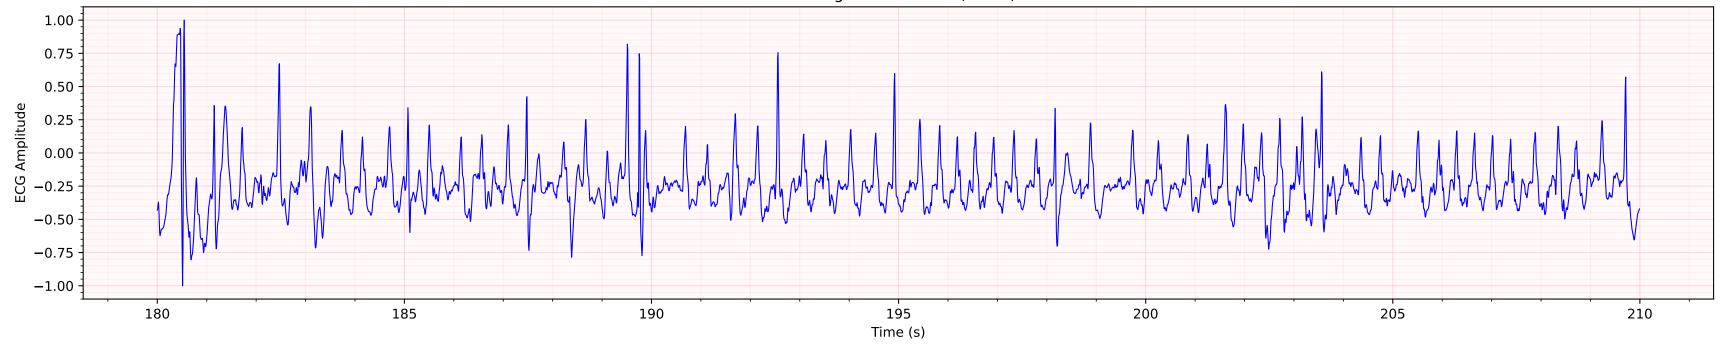


ECG Signal - Minute 4 (30-60s)

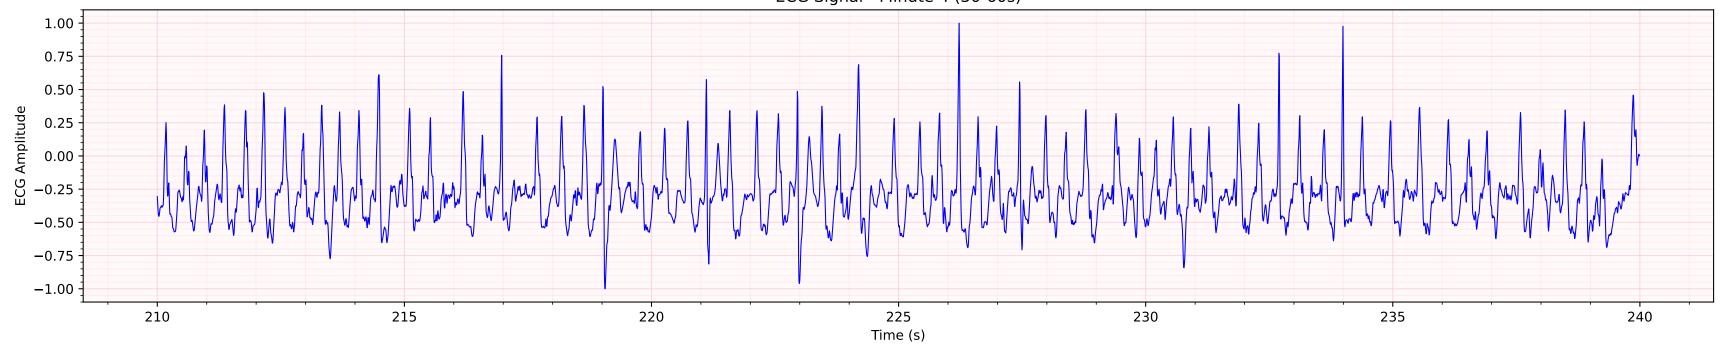


ECG Signal - Minute 5 (0-30s)

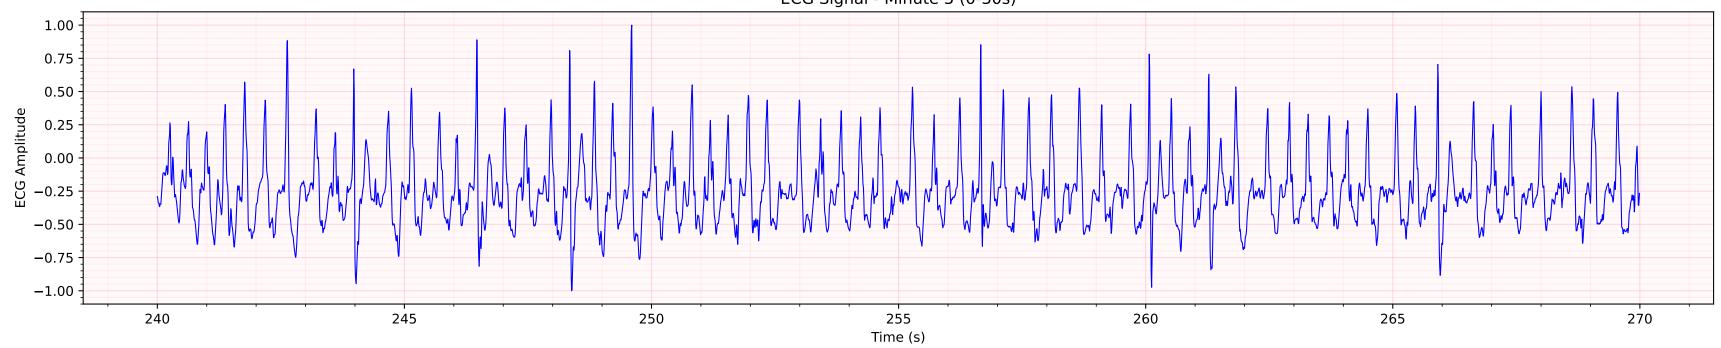


ECG Signal - Minute 5 (30-60s)

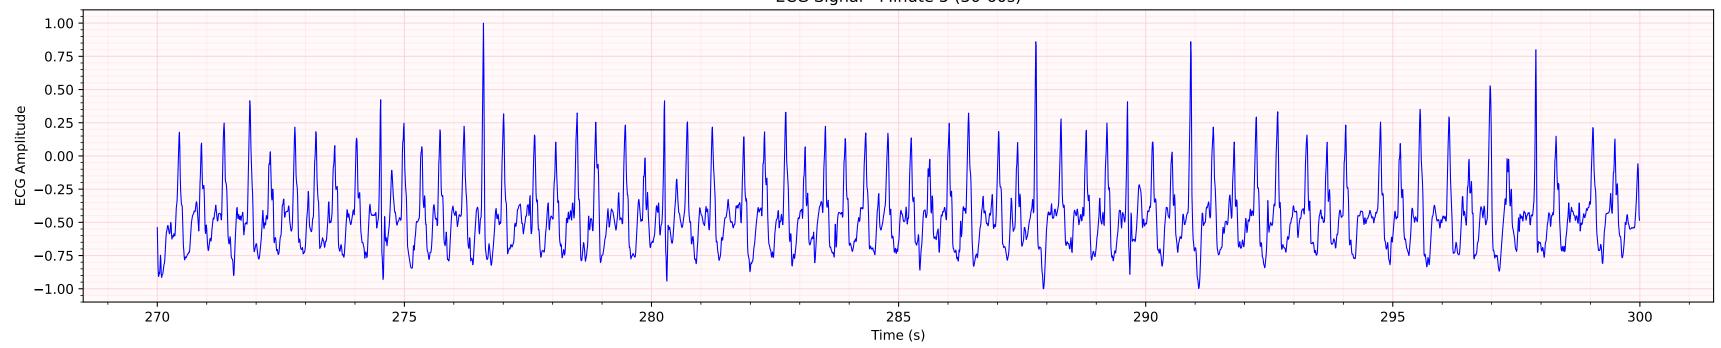

ECG Signal - Minute 6 (0-30s) 1.00 0.75 0.50

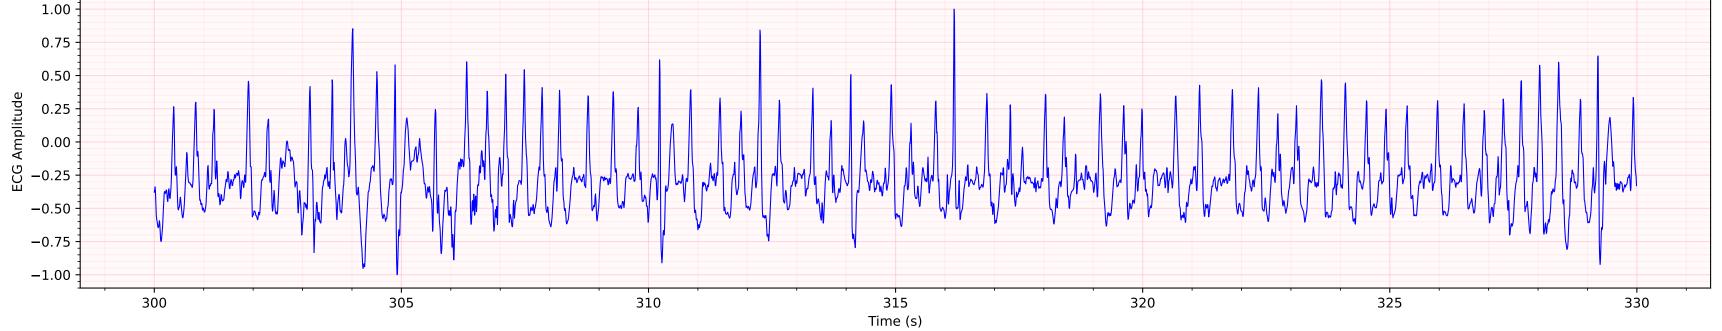

ECG Signal - Minute 6 (30-60s) 1.00 0.75 0.50

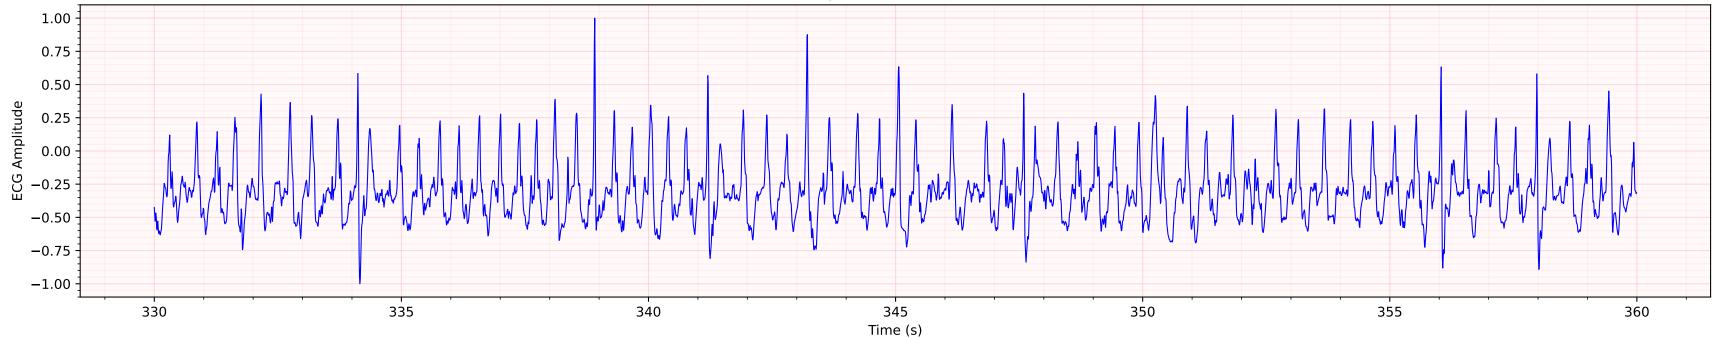

ECG Signal - Minute 7 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ −0.25 · -0.50 --0.75-1.00 ·

375

Time (s)


380

370


360

365


ECG Signal - Minute 7 (30-60s) 1.00 0.75 0.50

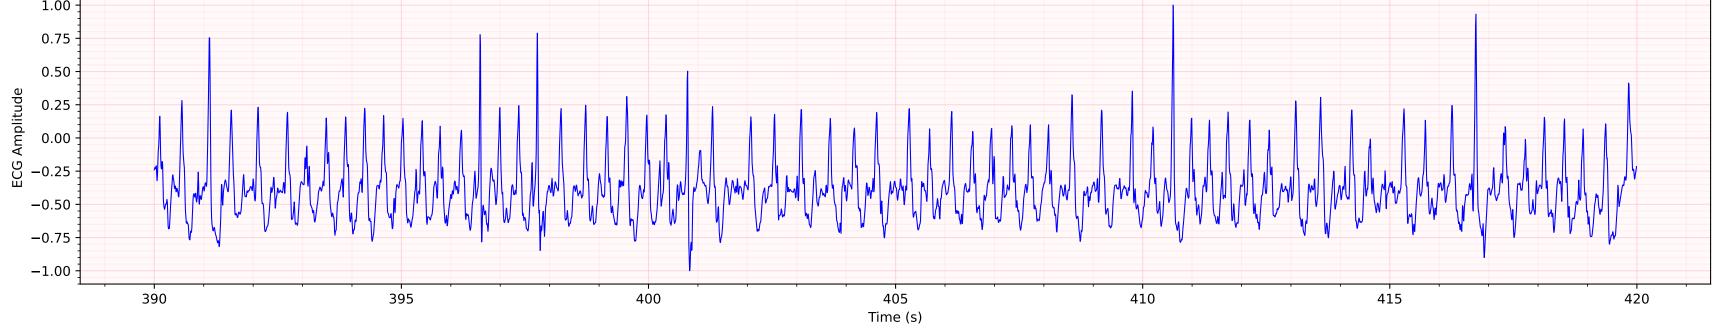


ECG Signal - Minute 8 (0-30s) 1.00 0.75 0.50

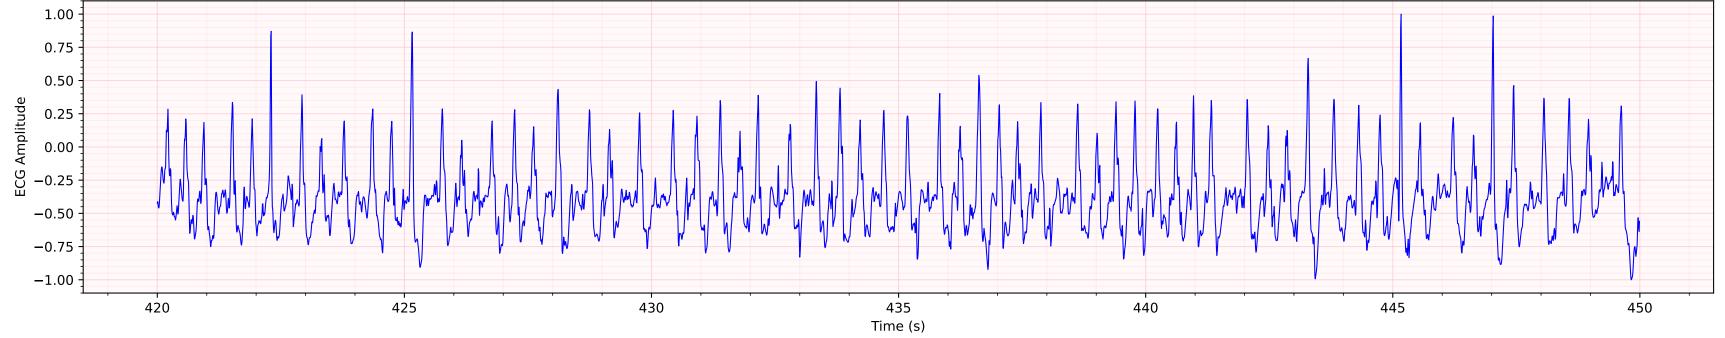

ECG Signal - Minute 8 (30-60s) 1.00

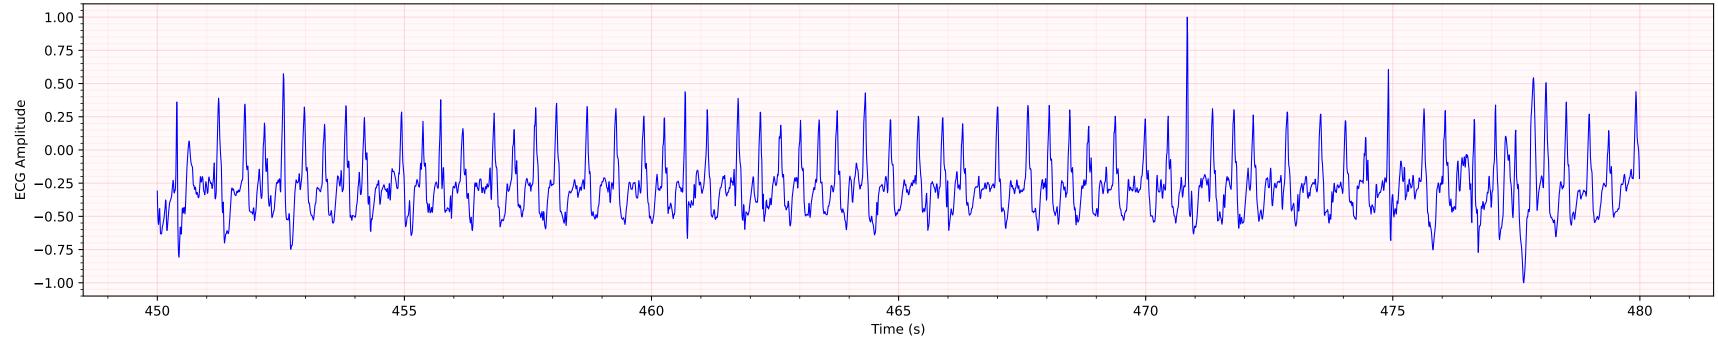


ECG Signal - Minute 9 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 -<u>0</u> -0.25

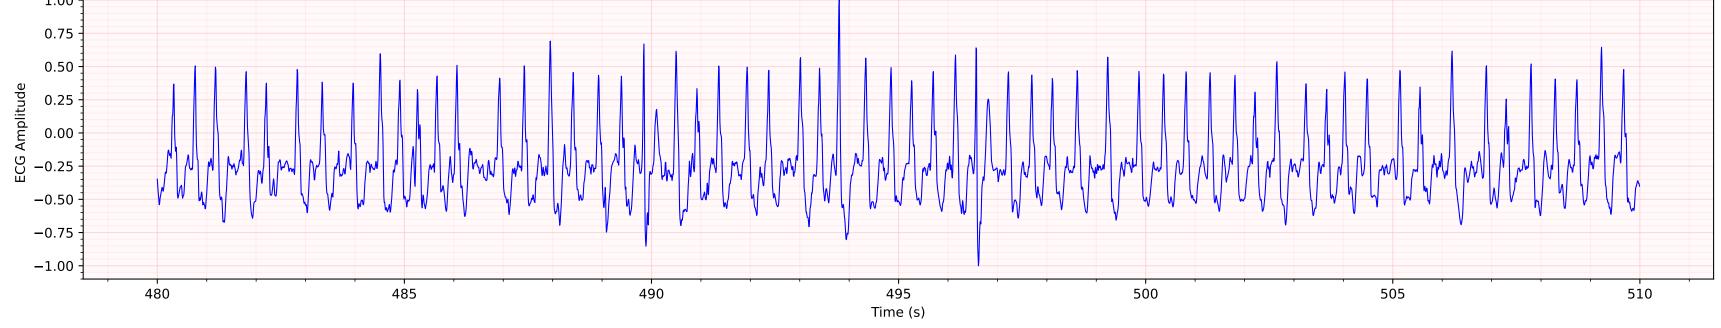


ECG Signal - Minute 9 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 <u>0</u> -0.25 -0.50 --0.75-1.00 · 510 515 520 525 530 535 540

ECG Signal - Minute 10 (0-30s) 1.00 0.75 0.50 Amplitude 0.00

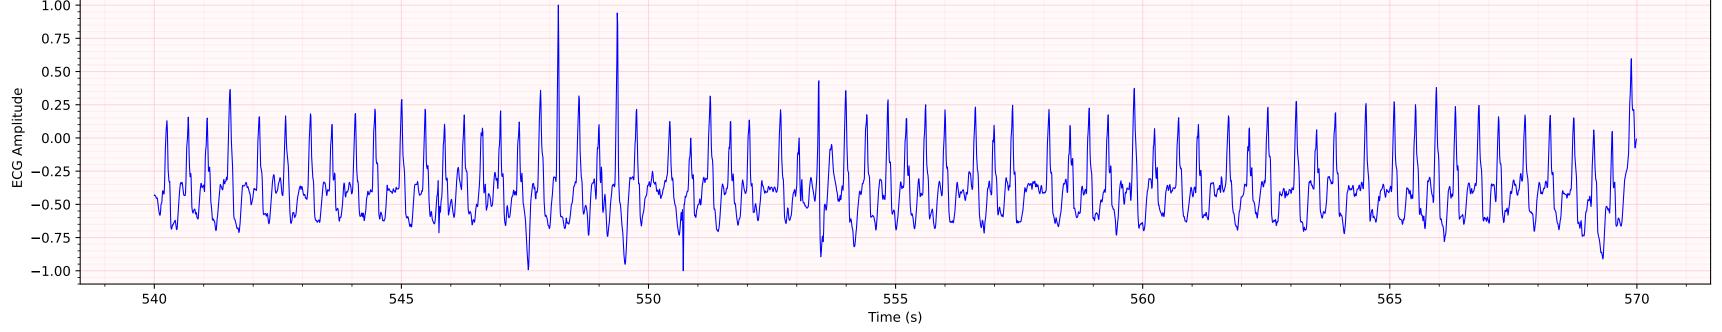


ECG Signal - Minute 10 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 უ −0.25 -0.50 · -0.75-1.00 -570 575 580 585 590 595 600 Time (s)

ECG Signal - Minute 11 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 უ −0.25

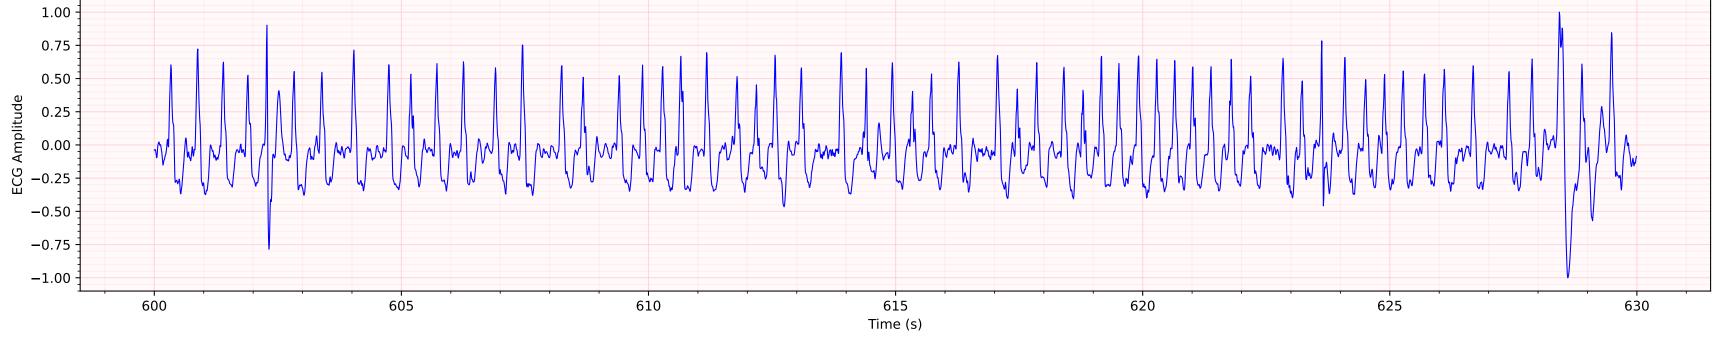


ECG Signal - Minute 11 (30-60s) 1.00 0.75 0.50 0.00 - Amplitude ⊕ −0.25 -0.50 -0.75-1.00 -630 635 640 650 655 660 645


ECG Signal - Minute 12 (0-30s) 1.00 0.75 0.50

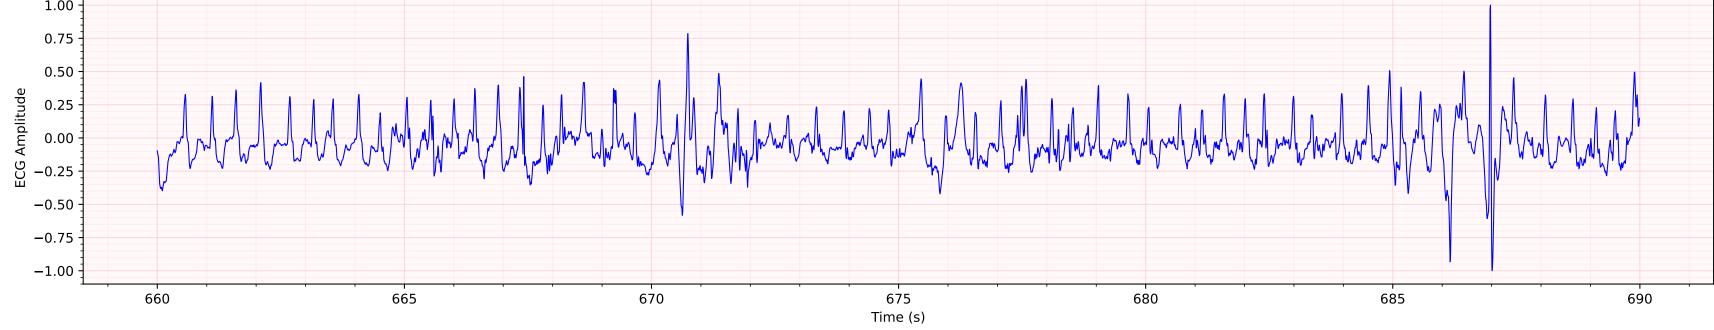

ECG Signal - Minute 12 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 <u>0</u> –0.25

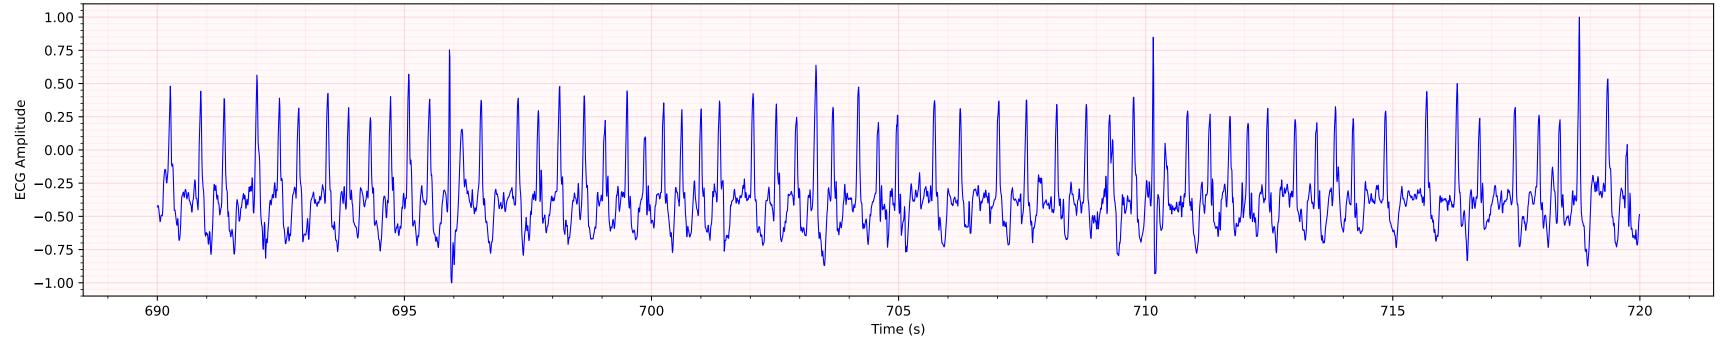


ECG Signal - Minute 13 (0-30s)

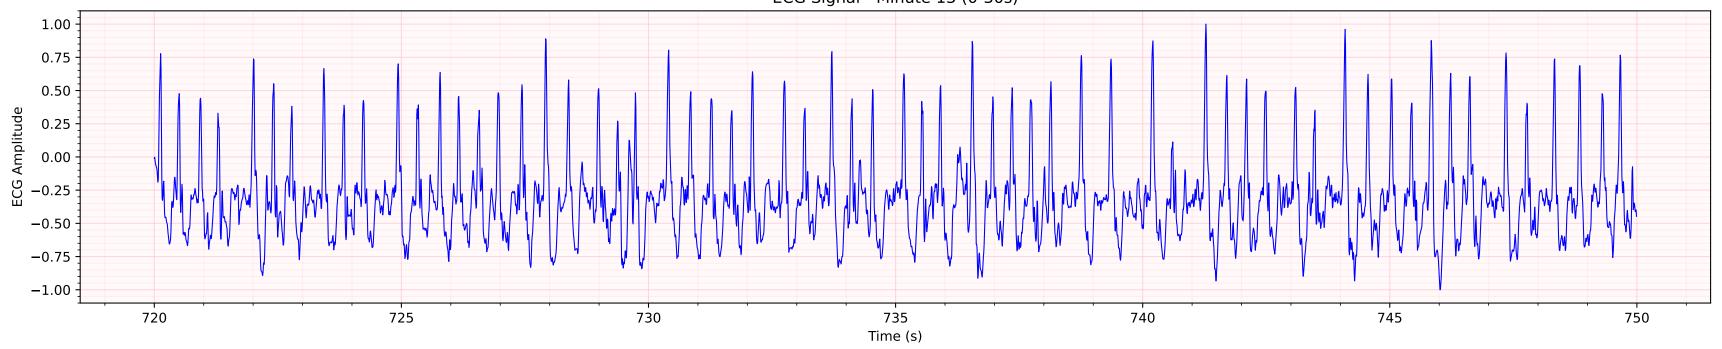


ECG Signal - Minute 13 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 · -0.75-1.00 -750 755 760 765 770 775


ECG Signal - Minute 14 (0-30s)

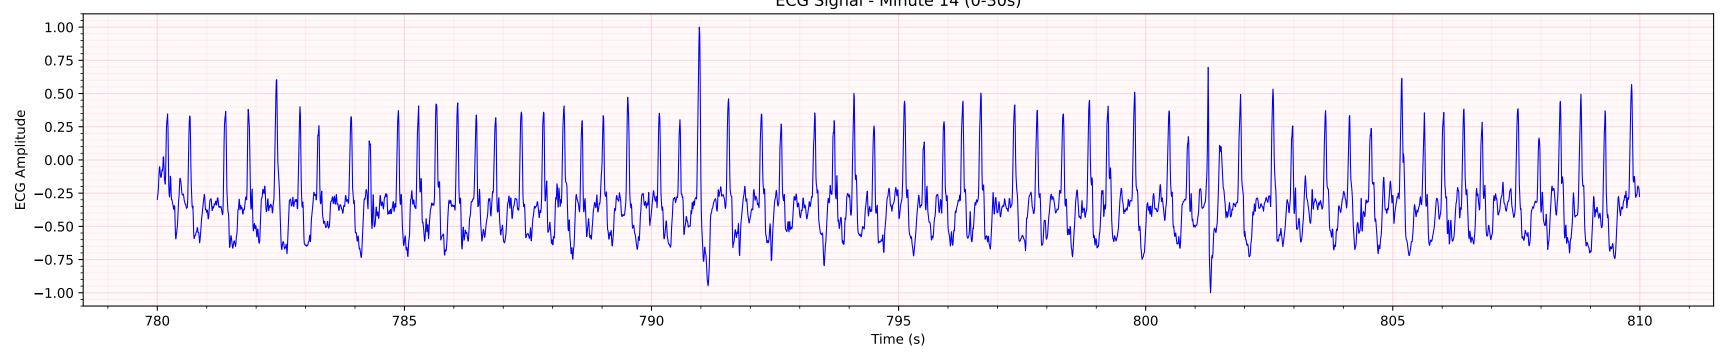

ECG Signal - Minute 14 (30-60s) 1.00 0.75 0.50

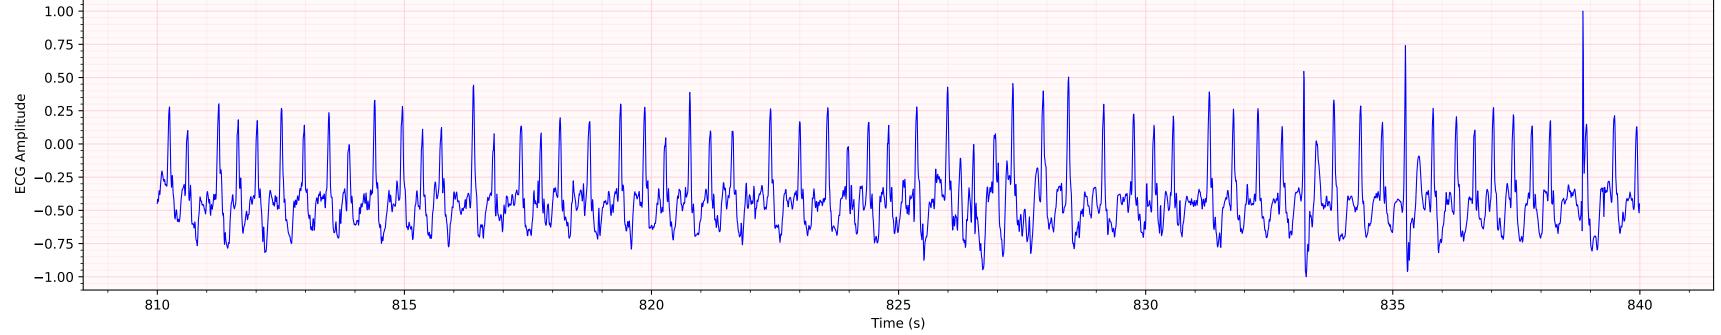

ECG Signal - Minute 15 (0-30s)

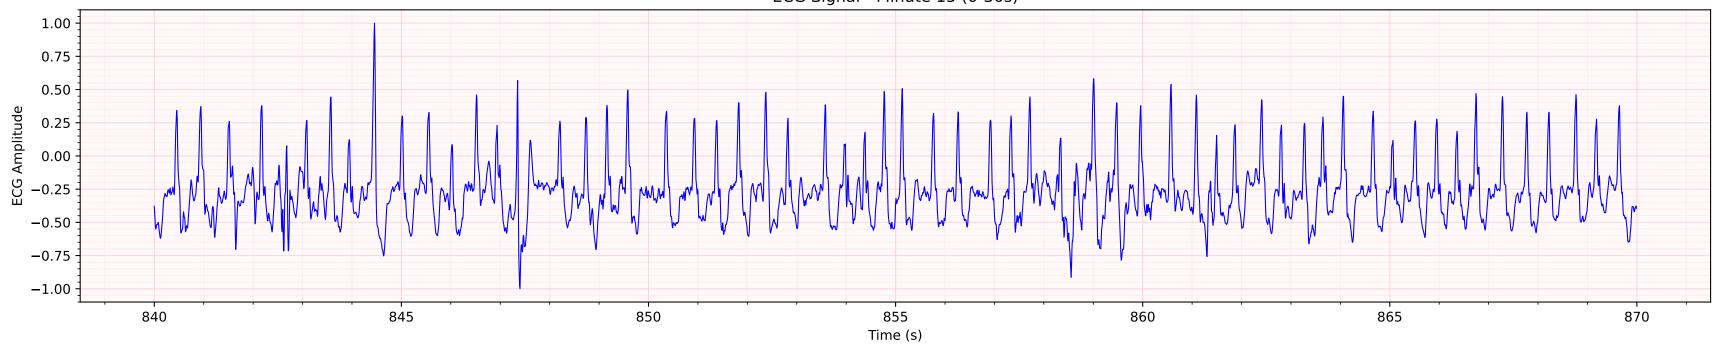

ECG Signal - Minute 15 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 --0.75-1.00870 875 880 890 895 885

ECG Signal - Minute 16 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 --0.75

920

925

930

-1.00

900

905

ECG Signal - Minute 16 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 = -0.50-0.75 · -1.00 ·

950

955


960

940

930

ECG Signal - Minute 17 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ −0.25 -0.50 · -0.75-1.00 · 960 965 970 980 985 990 975 Time (s)

ECG Signal - Minute 17 (30-60s)

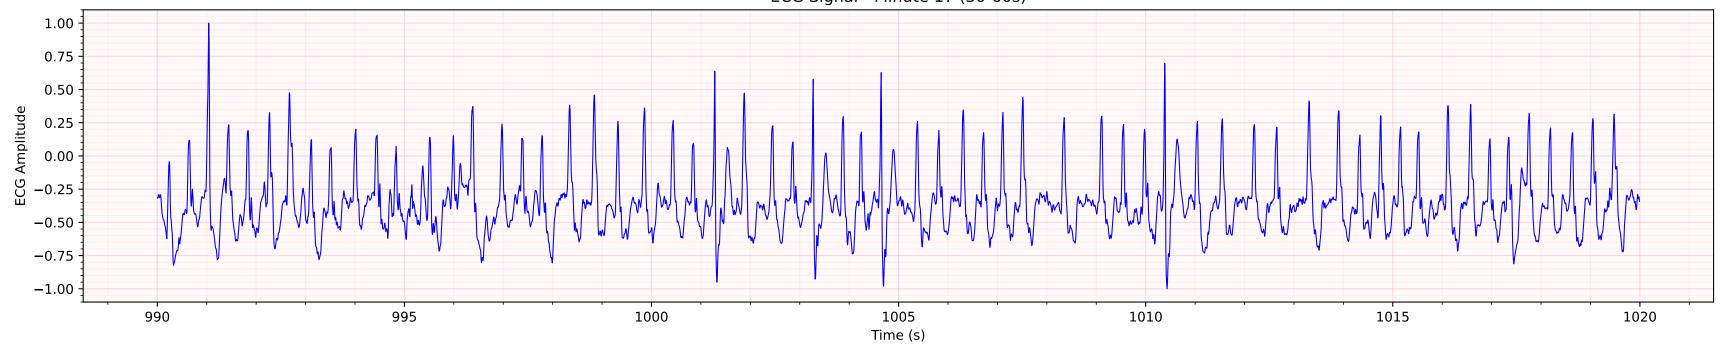

ECG Signal - Minute 18 (0-30s) 1.00 0.75 0.50 ECG Amplitude 0.00 --0.25 -0.50 = -0.50-0.75

1035

Time (s)

1045

1040


1050

1030


-1.00 -

1020


ECG Signal - Minute 18 (30-60s) 1.00 0.75 0.50

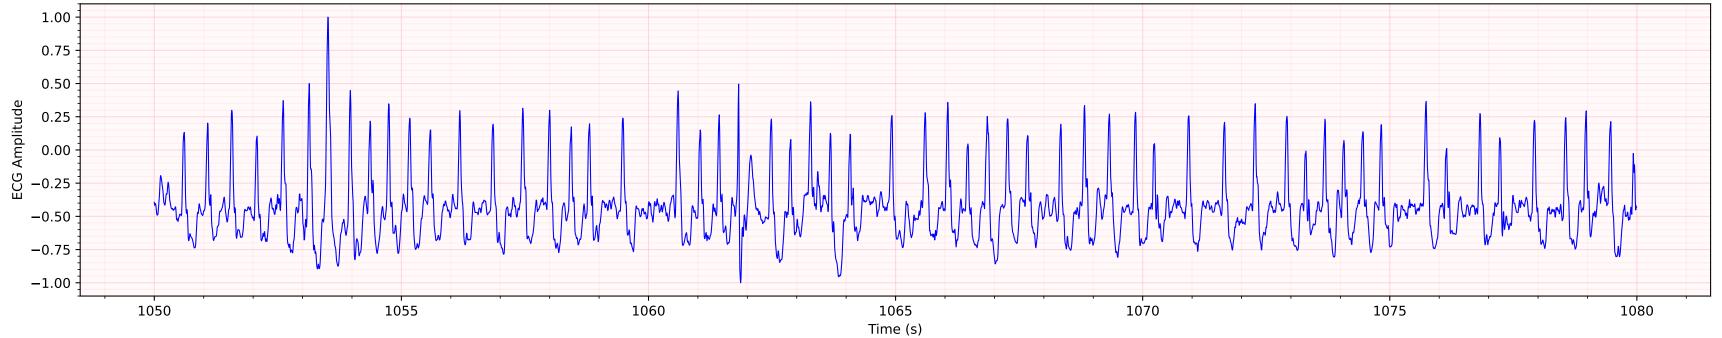


ECG Signal - Minute 19 (0-30s) 1.00 0.75 0.50

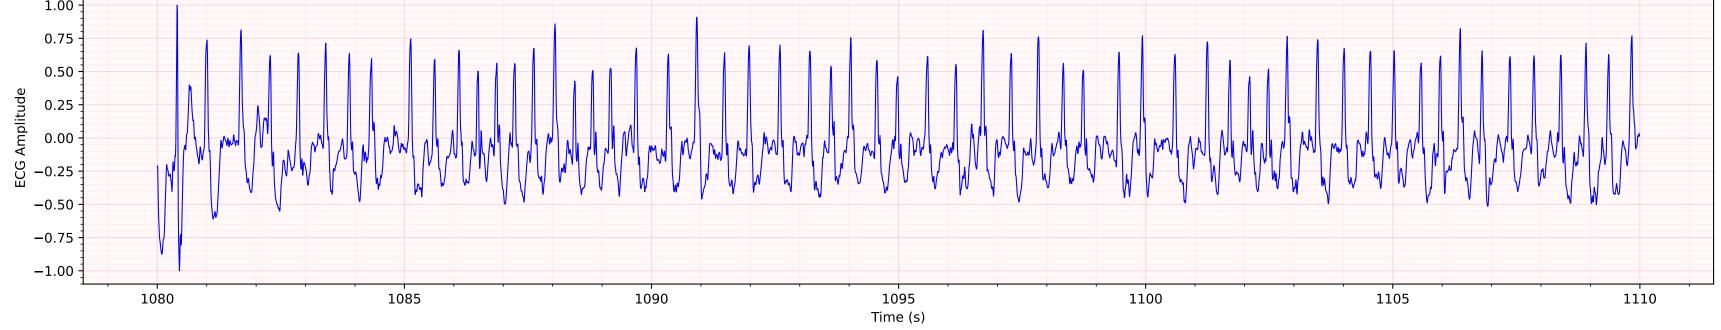

ECG Signal - Minute 19 (30-60s) 1.00 0.75 0.50 Amplitude 0.00

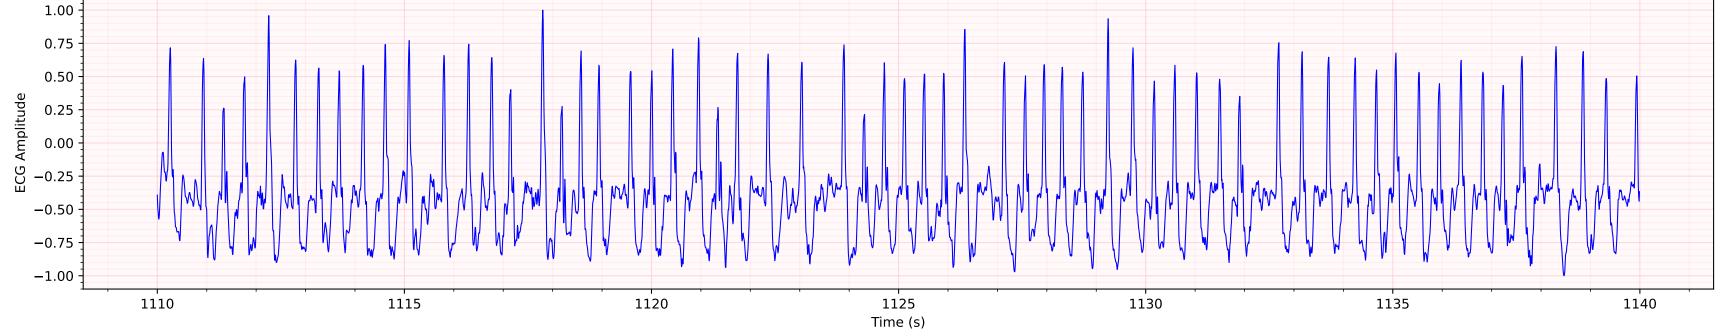

ECG Signal - Minute 20 (0-30s) 1.00 0.75 0.50

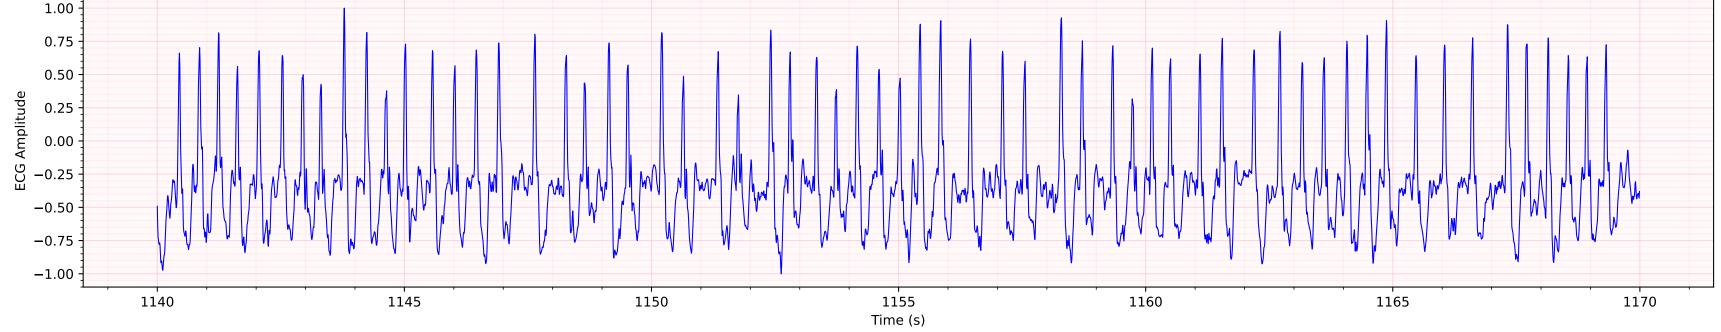

ECG Signal - Minute 20 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 <u>0</u> –0.25 -0.50 -

