


ECG Signal - Minute 1 (0-30s) 1.00 0.75 0.50 o.25 0.25 0.00 ⊕ –0.25 -0.50 · -0.75

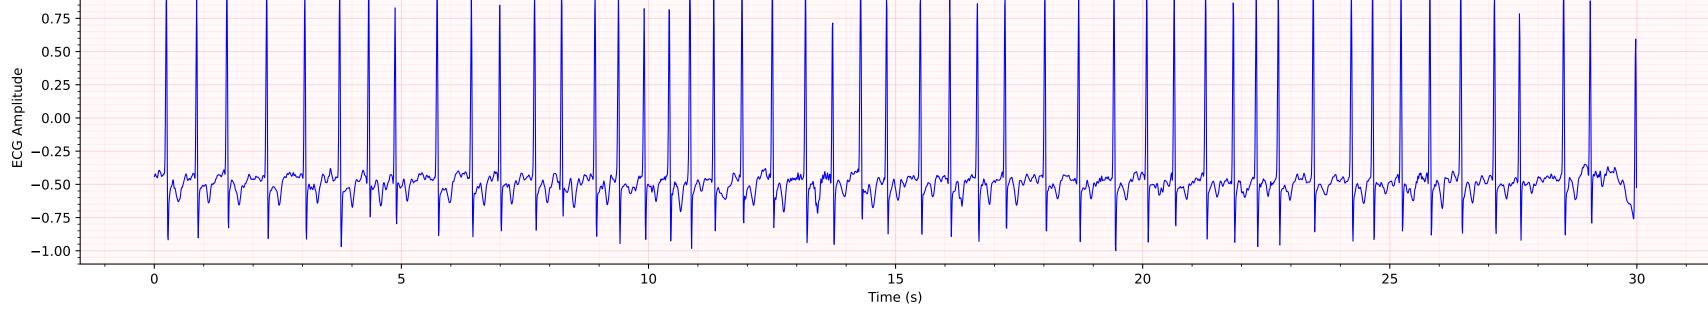

ECG Signal - Minute 1 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25

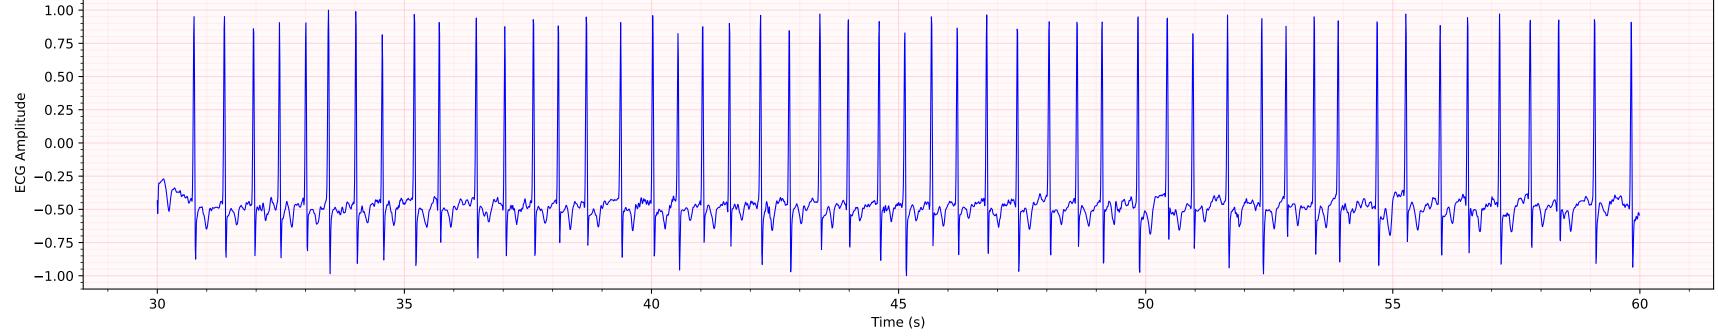


ECG Signal - Minute 2 (0-30s)

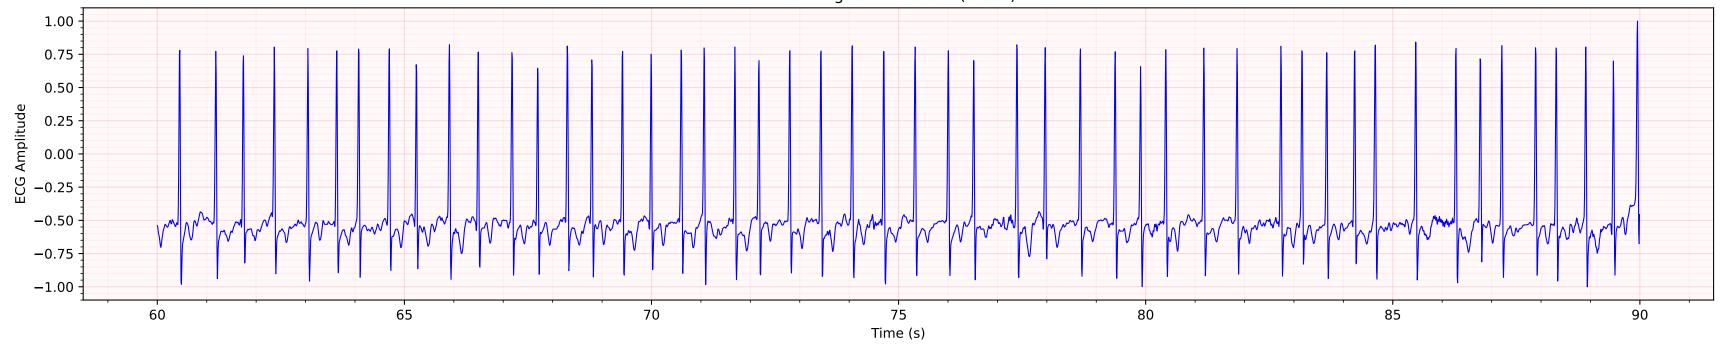


ECG Signal - Minute 2 (30-60s) 1.00 0.75 0.50 o.00 Amblitude ⊕ –0.25 -0.50 · -0.75 -1.0090 95 100 105 110 115 120


ECG Signal - Minute 3 (0-30s) 1.00 0.75 0.50

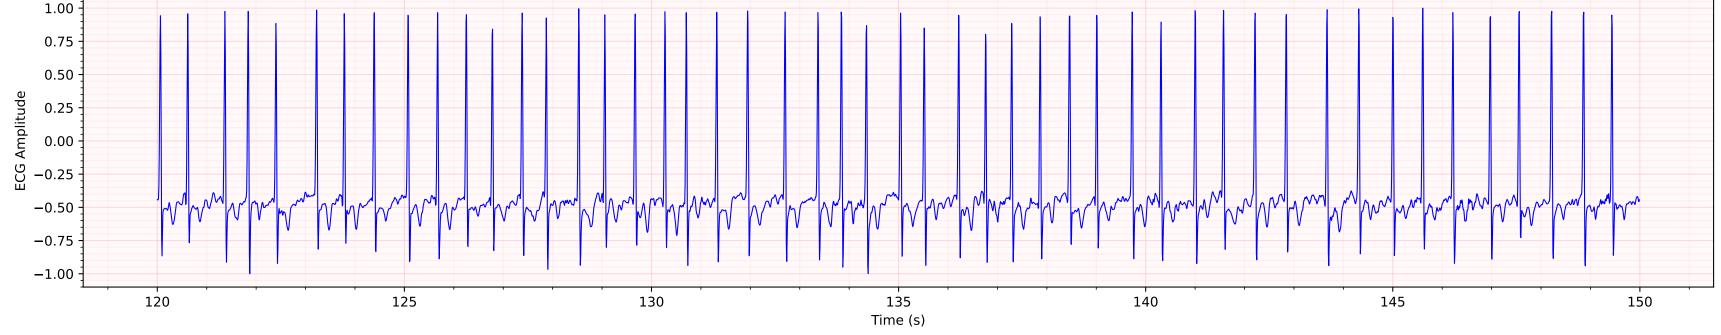


ECG Signal - Minute 3 (30-60s) 1.00 0.75 0.50

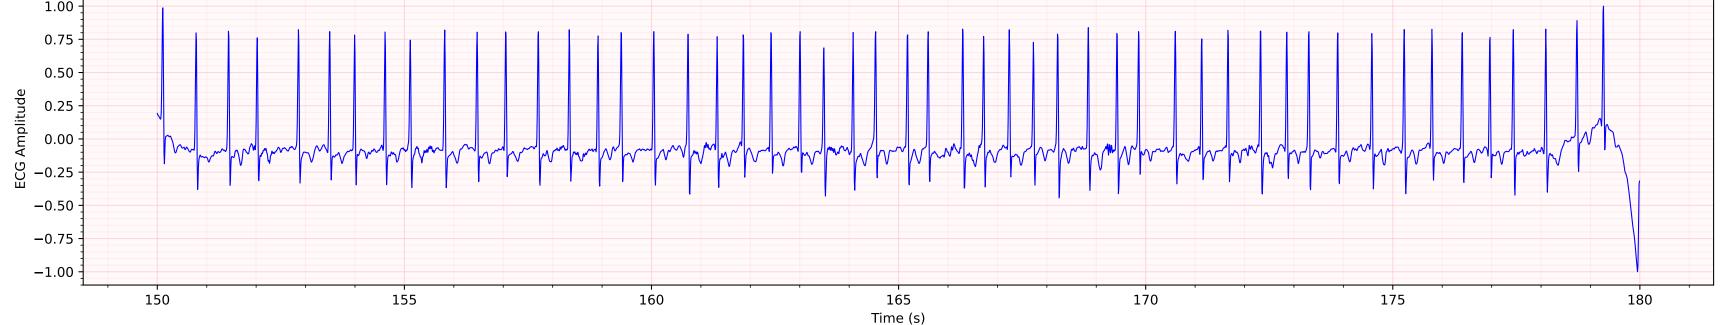

ECG Signal - Minute 4 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25

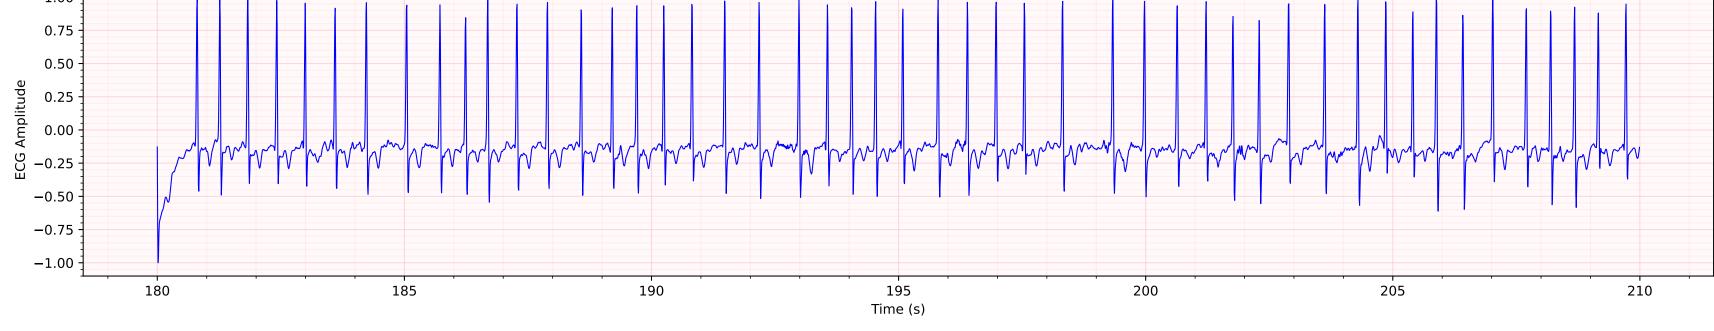

ECG Signal - Minute 4 (30-60s)

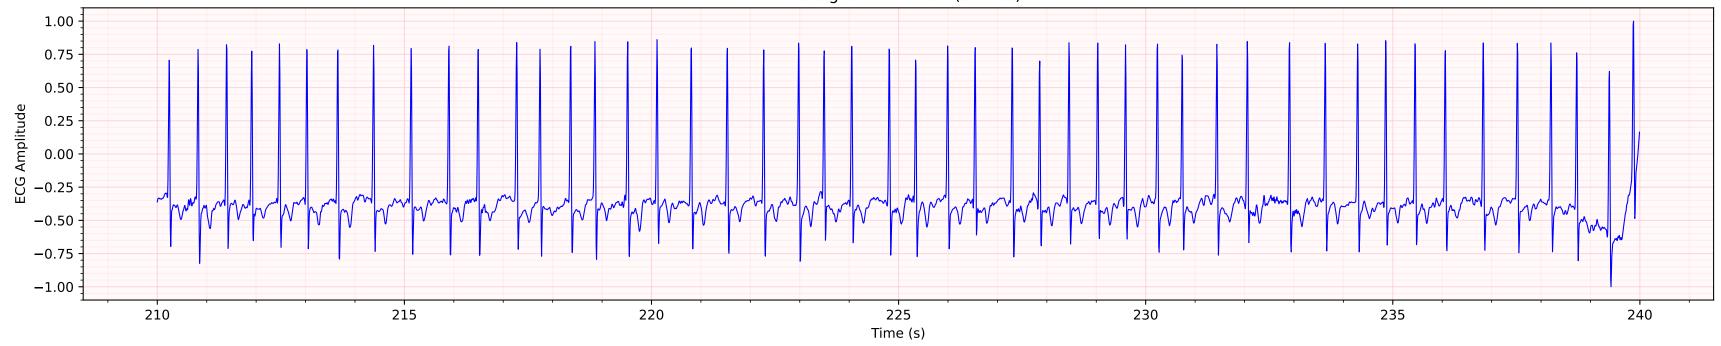

ECG Signal - Minute 5 (0-30s) 1.00 0.75 0.50 o.00 Amblitude ⊕ –0.25 -0.50 · -0.75 -1.00

255

Time (s)

265

260


270

250

240

245


ECG Signal - Minute 5 (30-60s)

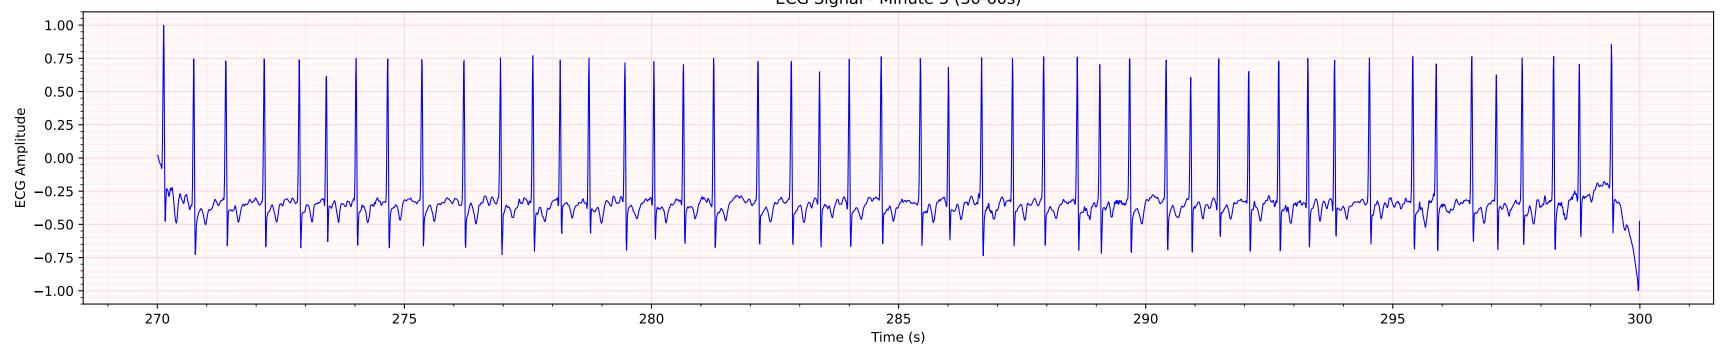

ECG Signal - Minute 6 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 · -0.75-1.00300 305 310 320 325 330 315 Time (s)

ECG Signal - Minute 6 (30-60s) 1.00 0.75 0.50 o.00 Amblitude ⊕ **–**0.25 -0.50 · -0.75-1.00330 335 340 345 350 355 360 Time (s)

ECG Signal - Minute 7 (0-30s)

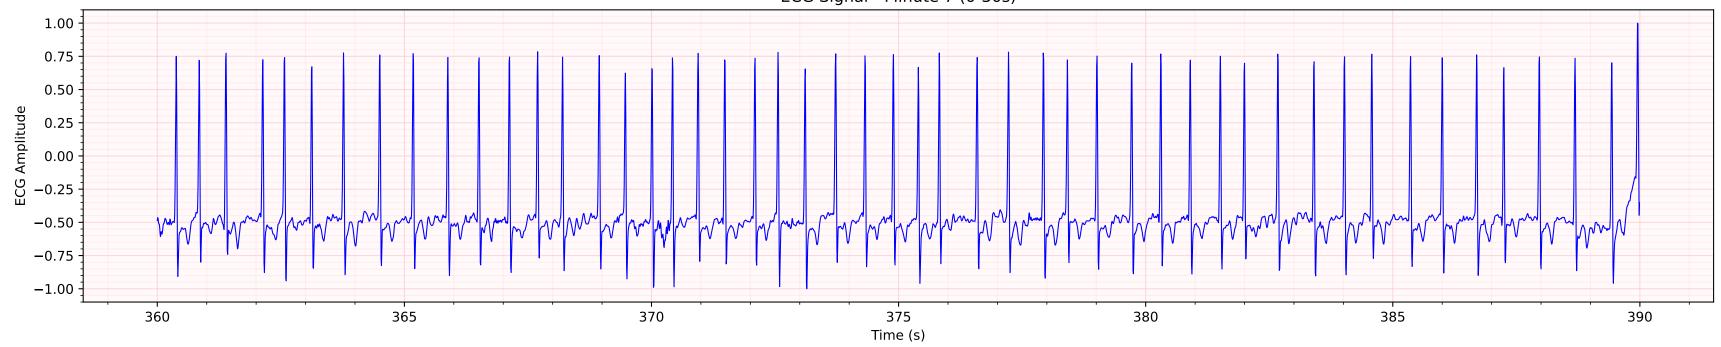

ECG Signal - Minute 7 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ **–**0.25 -0.50 · -0.75-1.00

405

Time (s)

410

415


400

420

390


395

ECG Signal - Minute 8 (0-30s) 1.00 0.75 0.50 Amplitude 0.00

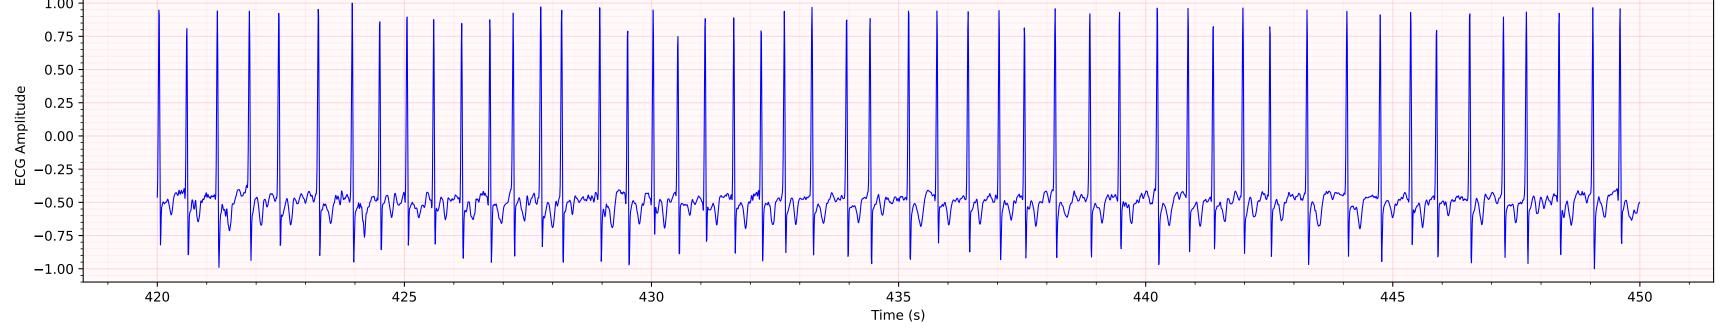


ECG Signal - Minute 8 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ **–**0.25 -0.50-0.75-1.00450 480 455 460 465 470 475

ECG Signal - Minute 9 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 · -0.75

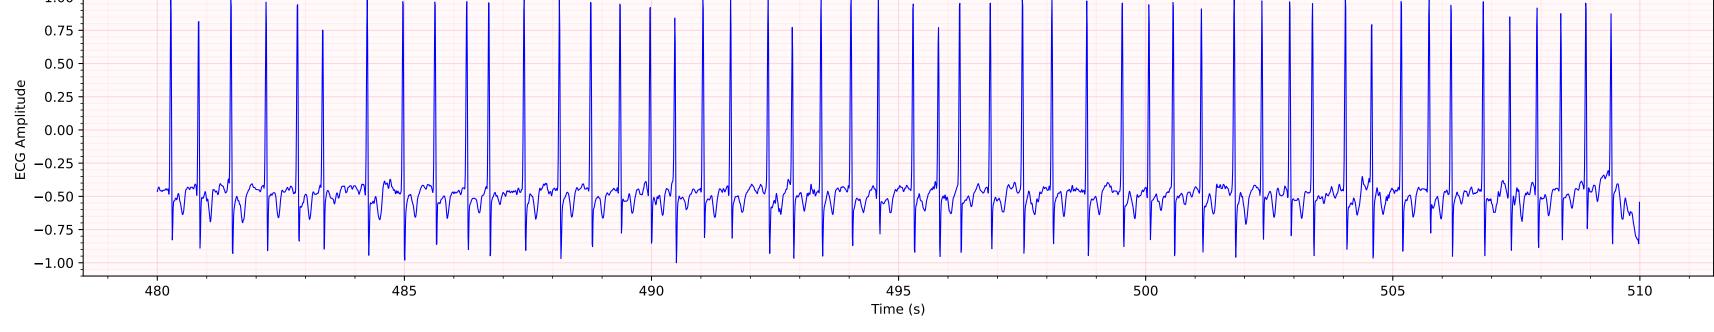


ECG Signal - Minute 9 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 $-0.50 = \frac{1}{2}$ -0.75-1.00510 520 525 535 540 515 530

ECG Signal - Minute 10 (0-30s) 1.00 0.75 0.50 Amplitude 0.00

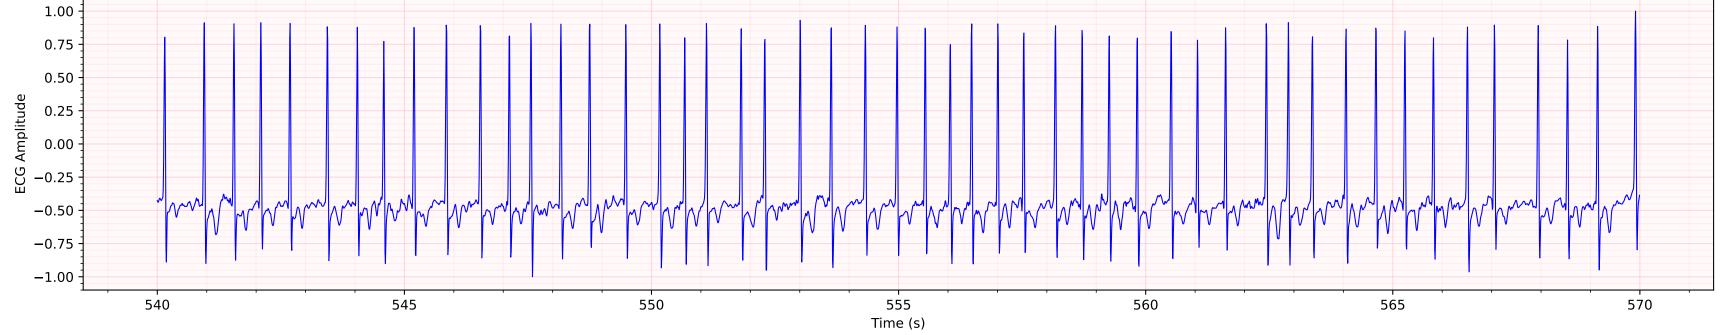


ECG Signal - Minute 10 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 · -0.75 -1.00570 575 580 585 590 595 600 Time (s)

ECG Signal - Minute 11 (0-30s)

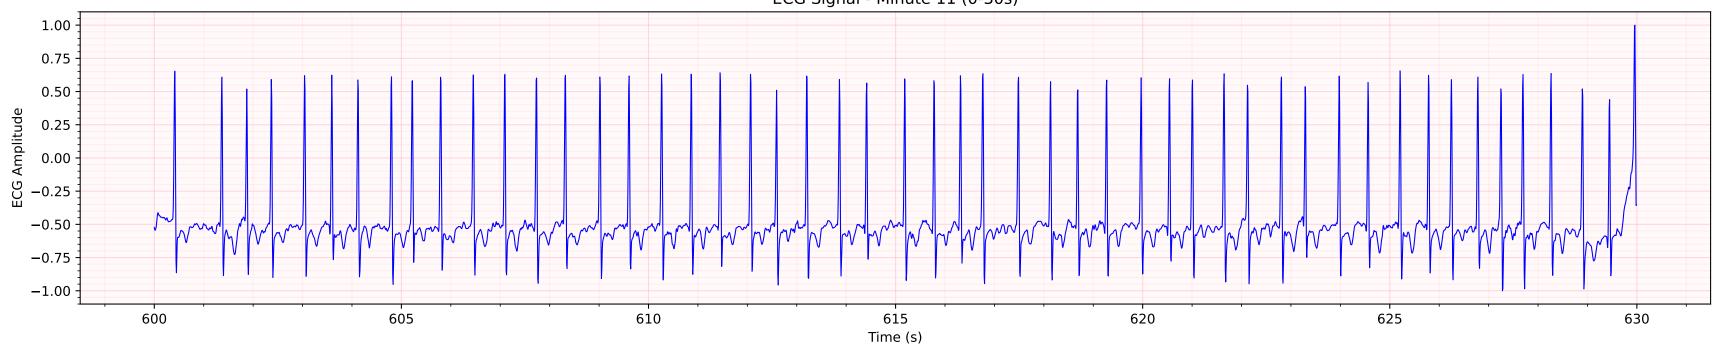


ECG Signal - Minute 11 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 · -0.75-1.00630 635 655 660 640 645 650 Time (s)


ECG Signal - Minute 12 (0-30s)

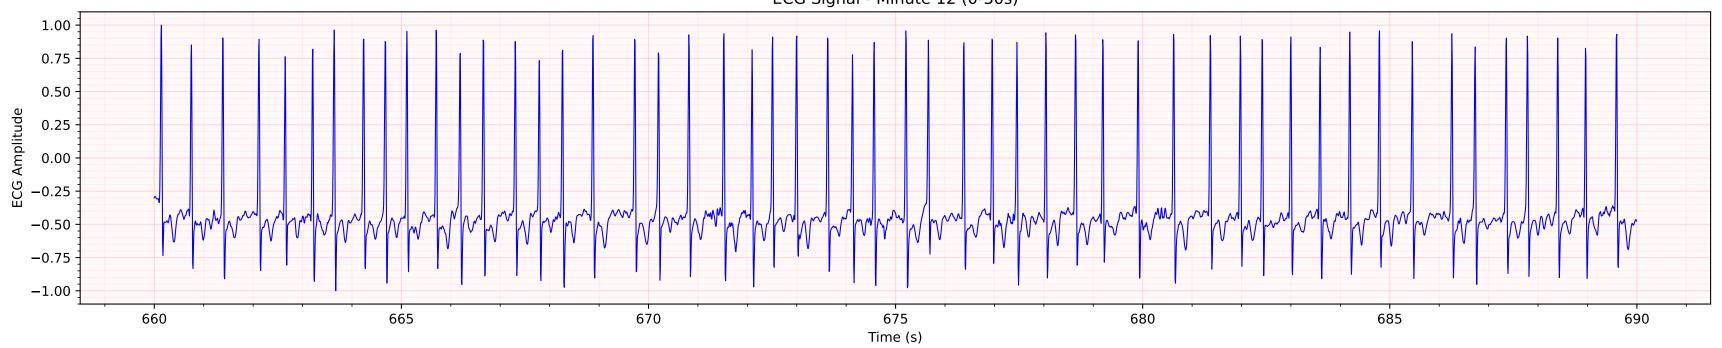

ECG Signal - Minute 12 (30-60s)

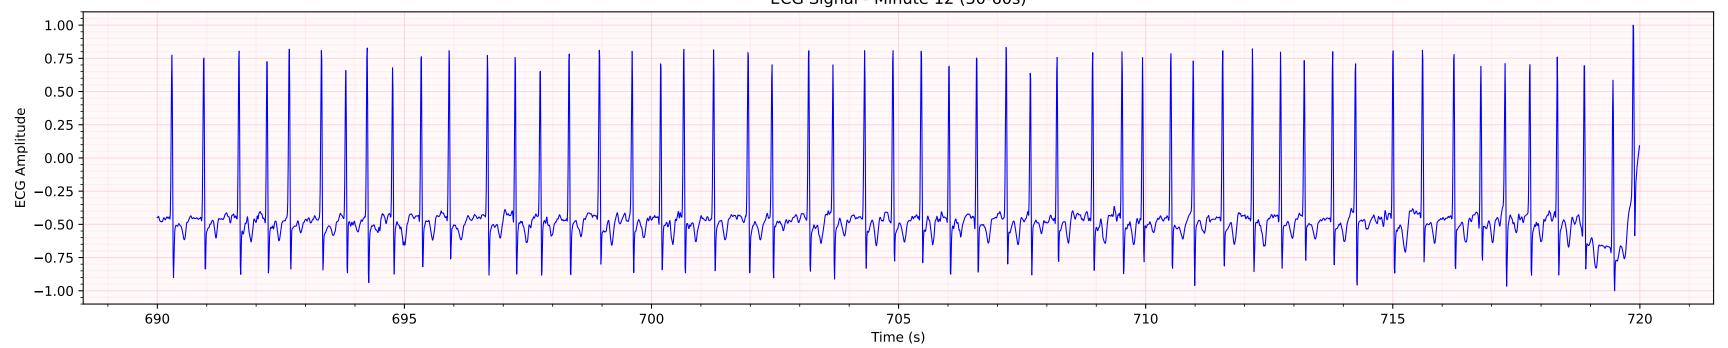


ECG Signal - Minute 13 (0-30s)

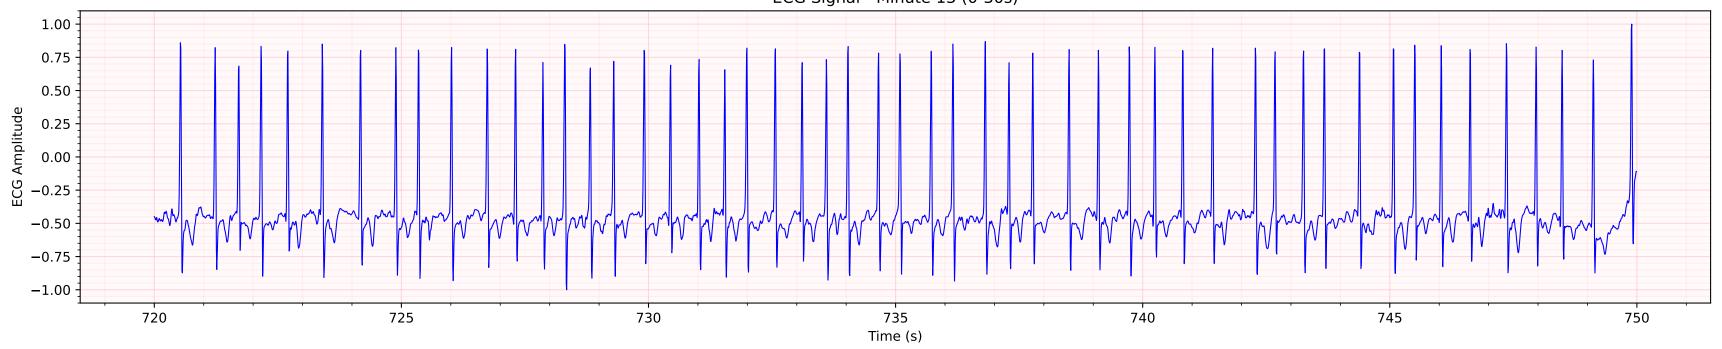

ECG Signal - Minute 13 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50-0.75 -1.00750 755 765 780 760 770 775 Time (s)

ECG Signal - Minute 14 (0-30s)

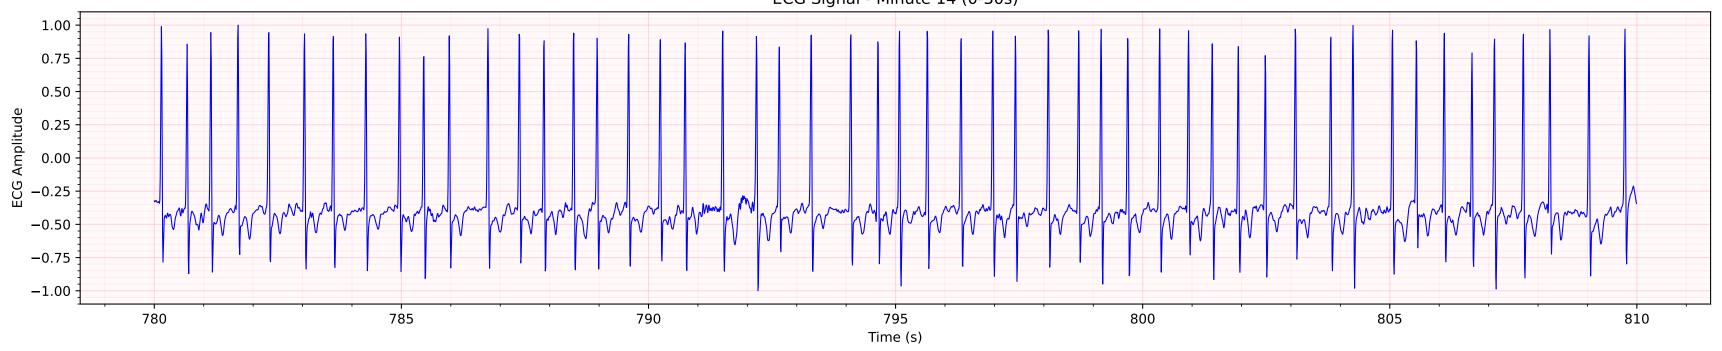


ECG Signal - Minute 14 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ **–**0.25 -0.50 · -0.75-1.00810 815 820 825 830 835 840 Time (s)

ECG Signal - Minute 15 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 -0.75-1.00840 850 865 870 845 855 860 Time (s)

ECG Signal - Minute 15 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 = -0.50-0.75-1.00870 875 880 895 900 885 890 Time (s)

ECG Signal - Minute 16 (0-30s)

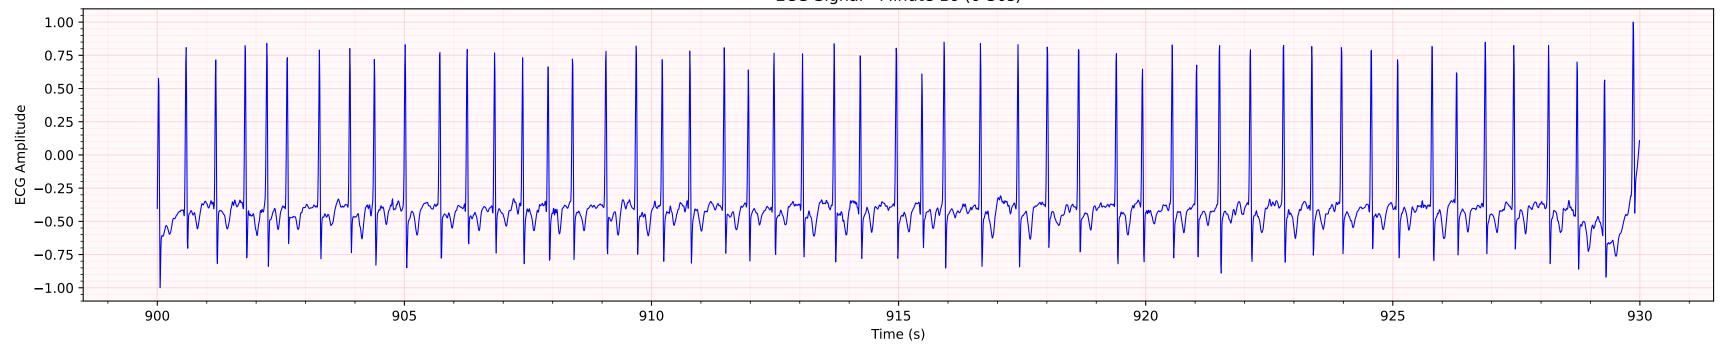


ECG Signal - Minute 16 (30-60s) 1.00 0.75 0.50 o.00 Amblitude ⊕ –0.25 -0.50-0.75 -1.00930 955 960 935 940 945 950 Time (s)

ECG Signal - Minute 17 (0-30s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 · -0.75-1.00960 985 990 965 970 975 980 Time (s)


ECG Signal - Minute 17 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ -0.25 -0.50 · -0.75-1.00990 995 1000 1015 1020 1005 1010

ECG Signal - Minute 18 (0-30s)

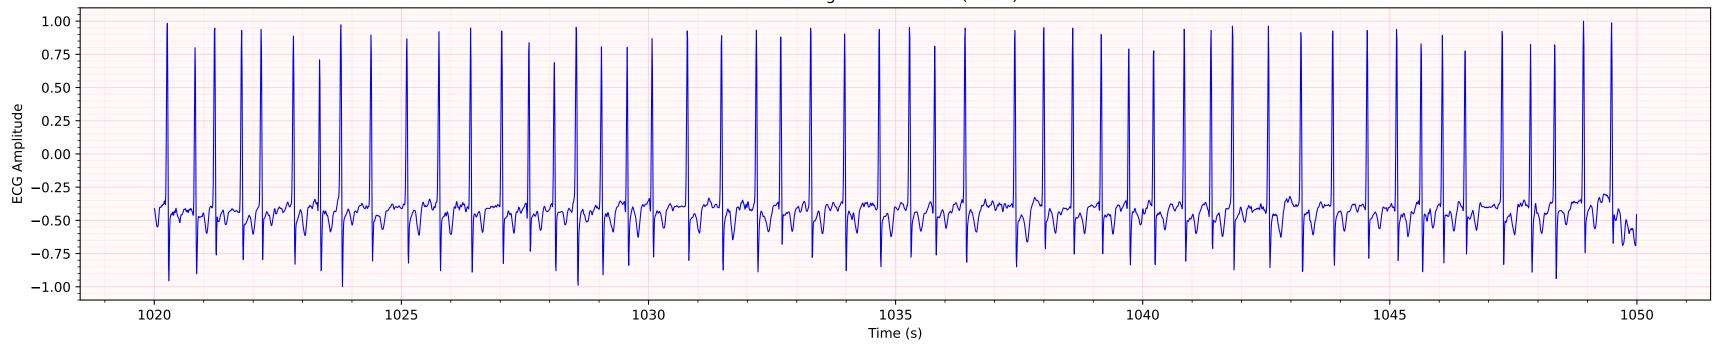

ECG Signal - Minute 18 (30-60s) 1.00 -0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50-0.75-1.001050 1075 1080 1055 1060 1065 1070 Time (s)

ECG Signal - Minute 19 (0-30s) 1.00 0.75 0.50

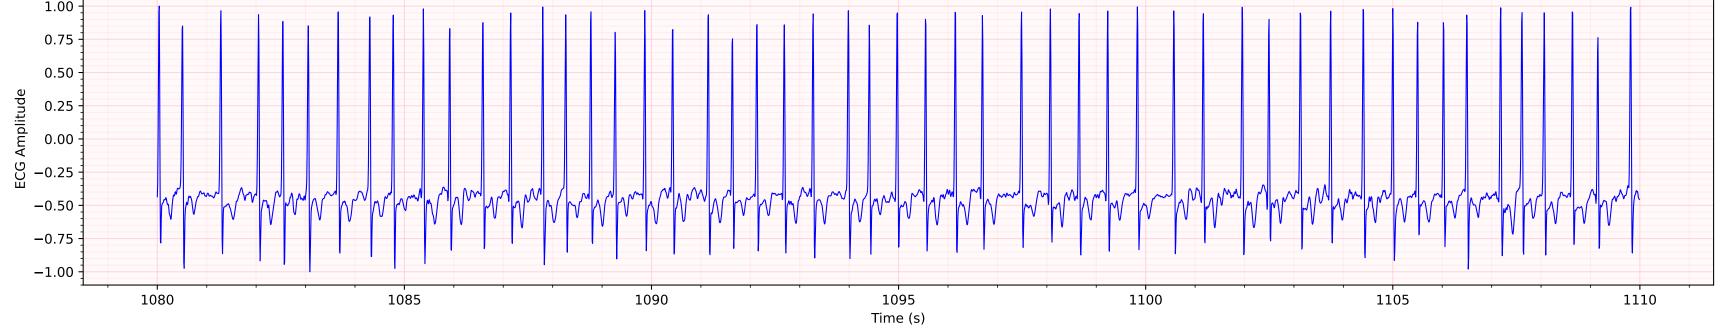

ECG Signal - Minute 19 (30-60s) 1.00 0.75 0.50 Amplitude 0.00 ⊕ –0.25 -0.50 · -0.75-1.00

1125

Time (s)

1130

1135


1140

1120

1110

1115

ECG Signal - Minute 20 (0-30s)

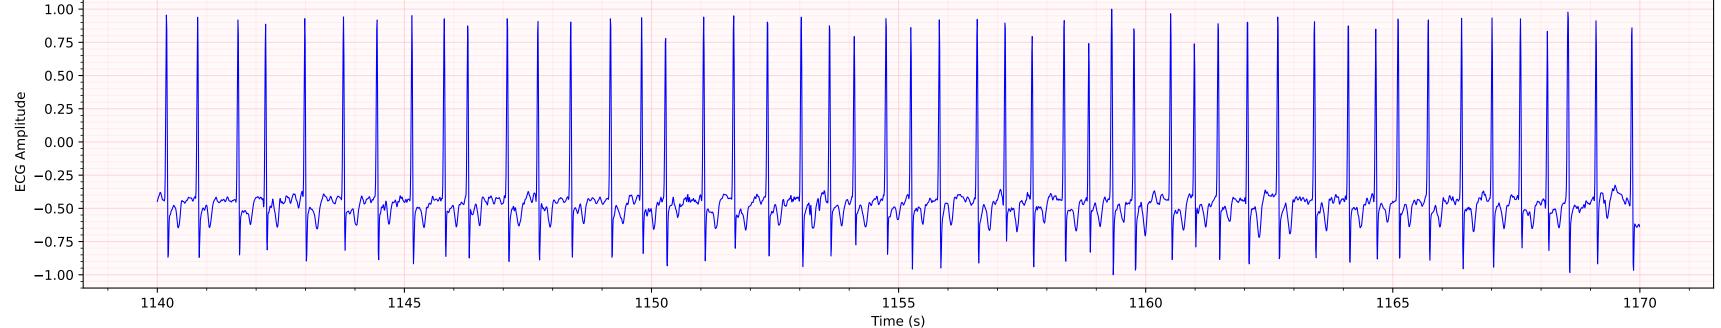

ECG Signal - Minute 20 (30-60s) 1.00 0.75 0.50 Amplitude 0.00

