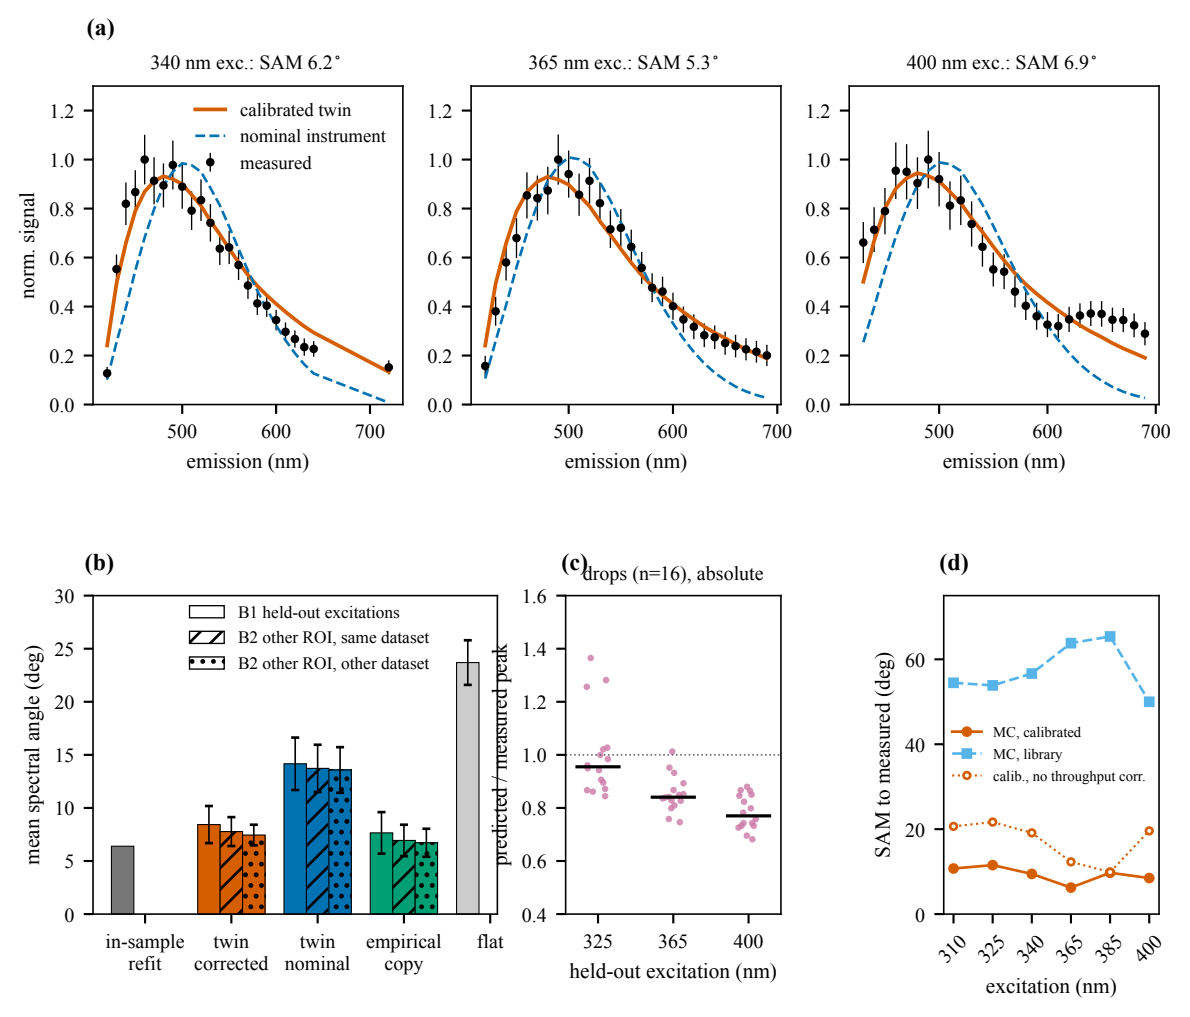

(a)
340 nm exc.: SAM 6.2°
365 nm exc.: SAM 5.3°
400 nm exc.: SAM 6.9°
calibrated twin
nominal instrument
measured
norm. signal
emission (nm)
(b)
B1 held-out excitations
B2 other ROI, same dataset
B2 other ROI, other dataset
mean spectral angle (deg)
in-sample refit
twin corrected
twin nominal
empirical copy
flat
(c)
drops (n=16), absolute
predicted / measured peak
held-out excitation (nm)
(d)
MC, calibrated
MC, library
calib., no throughput corr.
SAM to measured (deg)
excitation (nm)