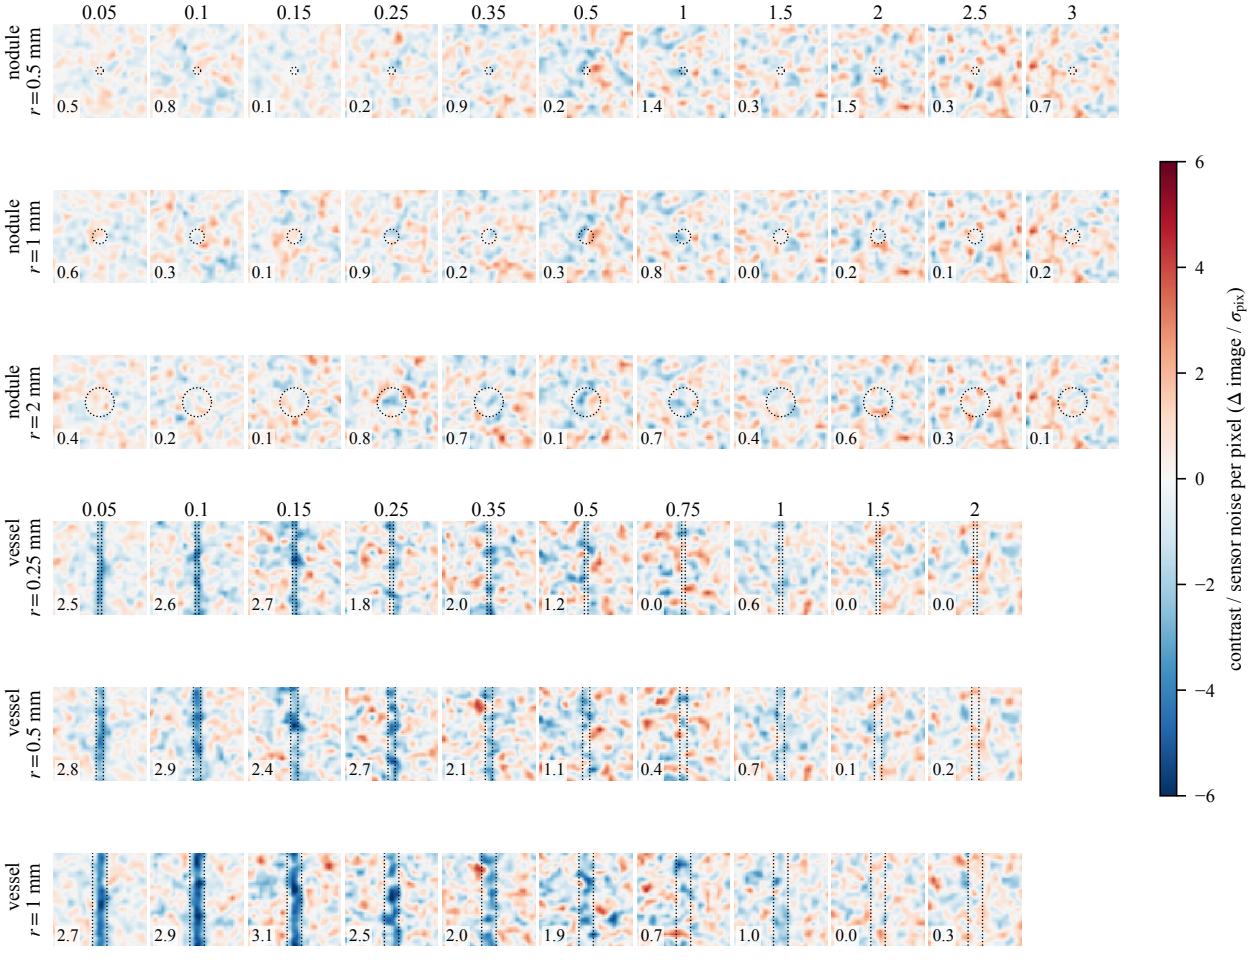


365 nm excitation, fluorescence bands, matched no-inclusion capture subtracted, mean of 3 MC seeds; column labels = depth d of the inclusion top (mm); white number = instrument CNR; dotted = true inclusion outline; tile = 11.5 mm