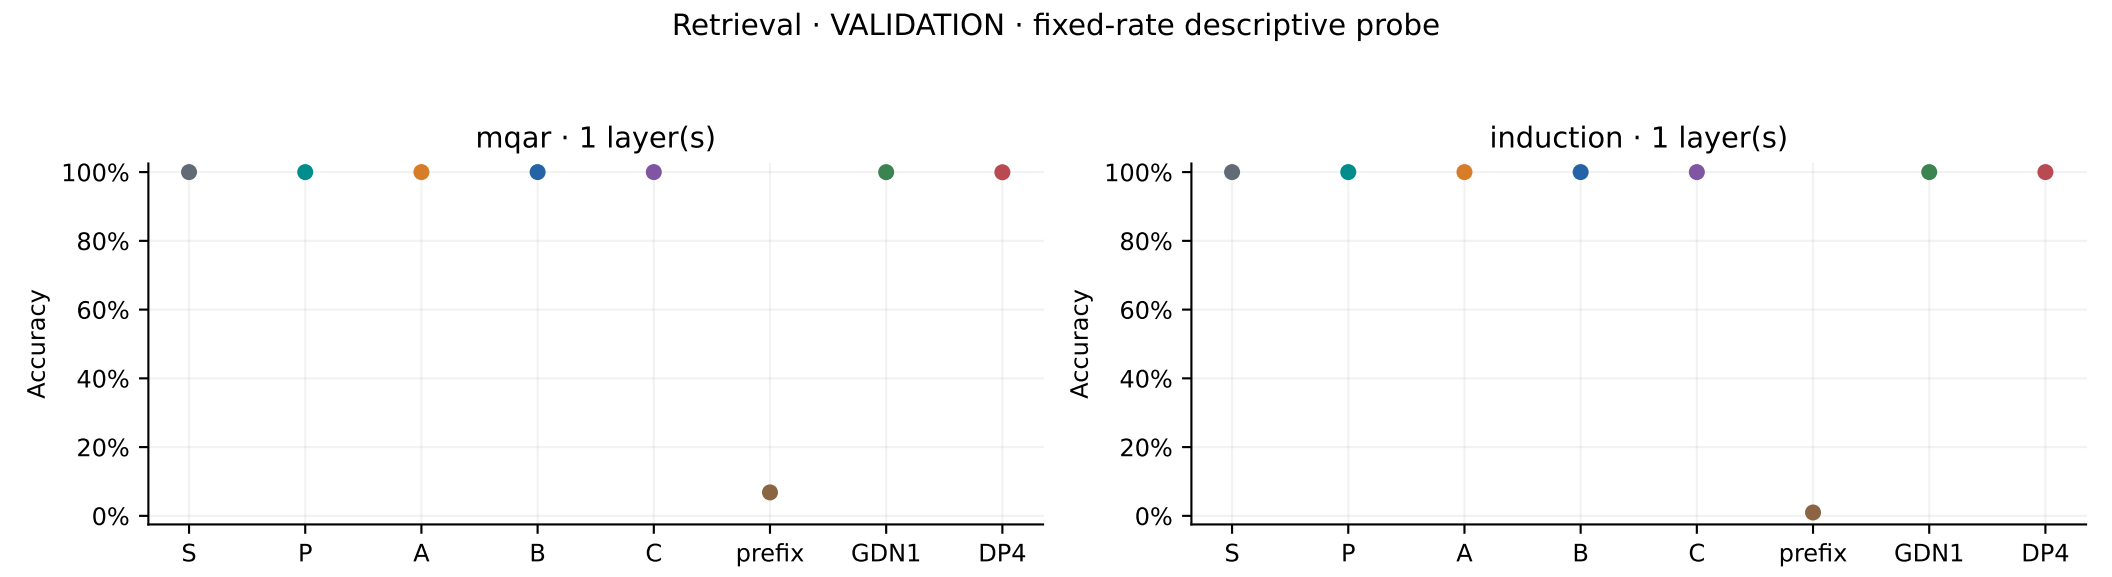
Retrieval · VALIDATION · fixed-rate descriptive probe
mqar · 1 layer(s)
induction · 1 layer(s)
Accuracy
100%
80%
60%
40%
20%
0%
S
P
A
B
C
prefix
GDN1
DP4
Each point is one run. Error bars are 1.96 × reported SE where available.