


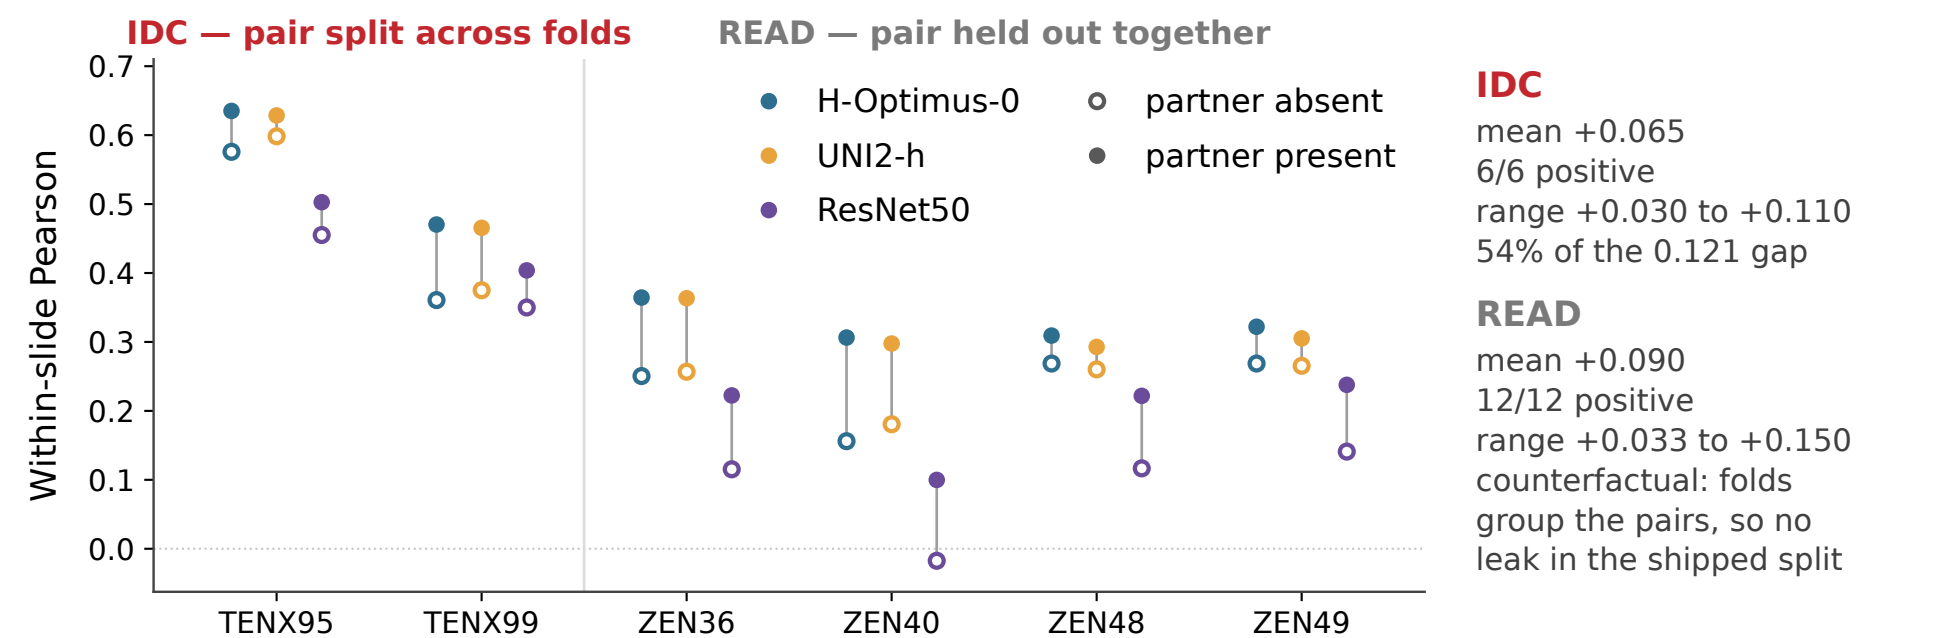

Test spots and training-set size held fixed within every pair; only the partner's availability varies. Positive in 18 of 18 encoder-slide cells, pooled mean +0.0818. Same-donor pairs established in results/round2/R5b_audit/ (IDC probable, unresolved; READ confirmed same specimen).