External GaAs quantum-dot data: useful interference contrast, conditional interpretation

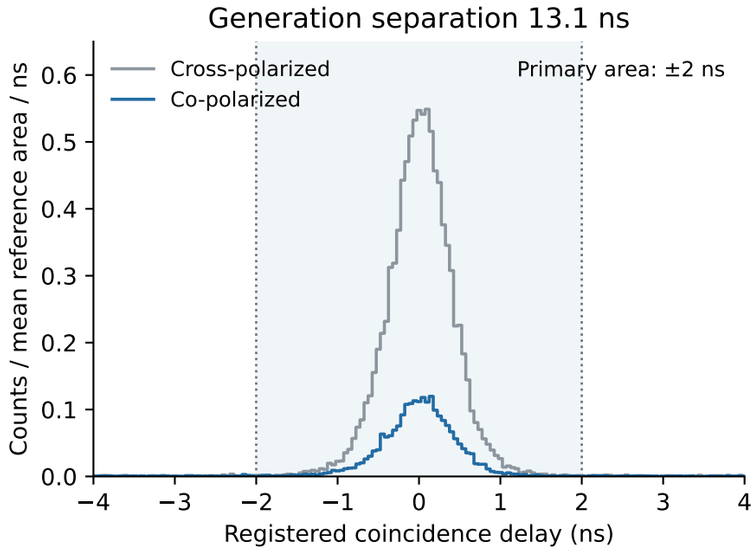

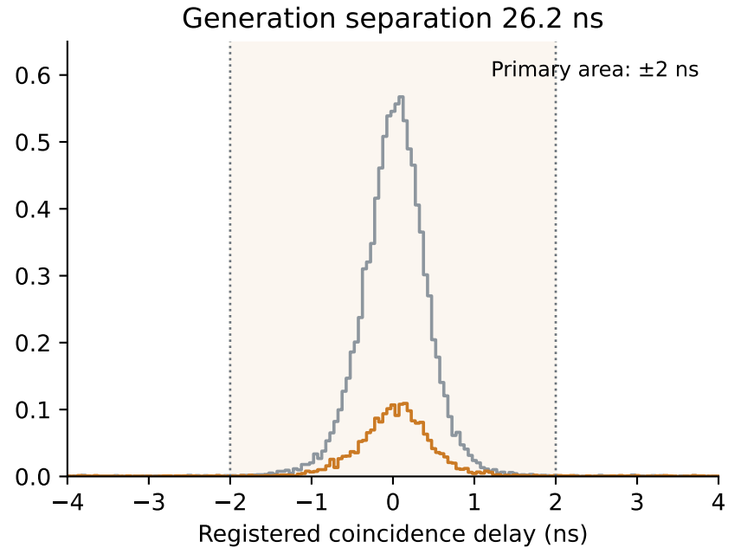

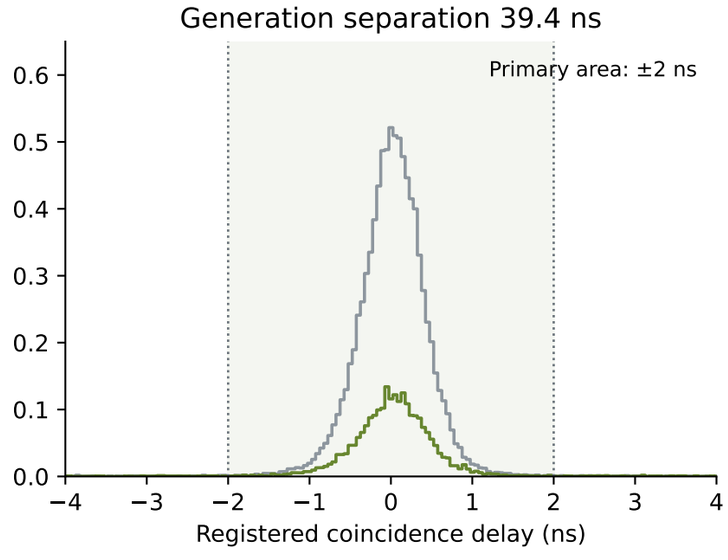

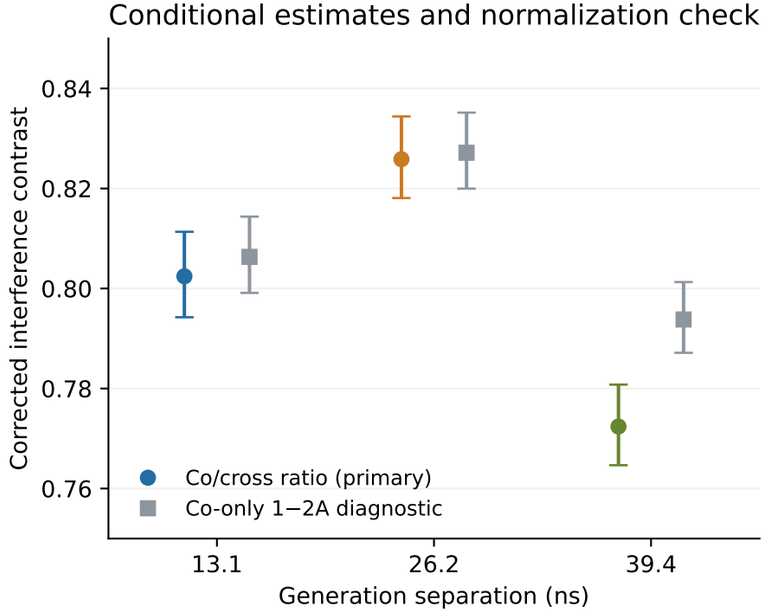

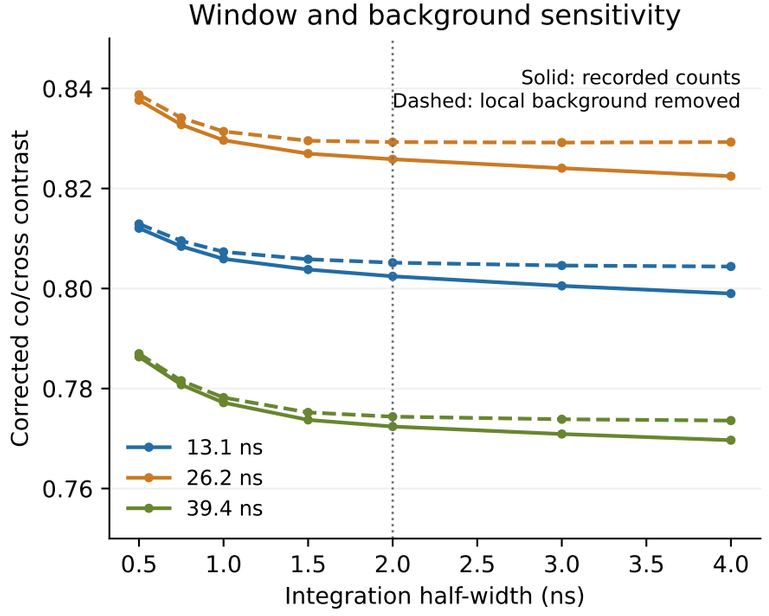

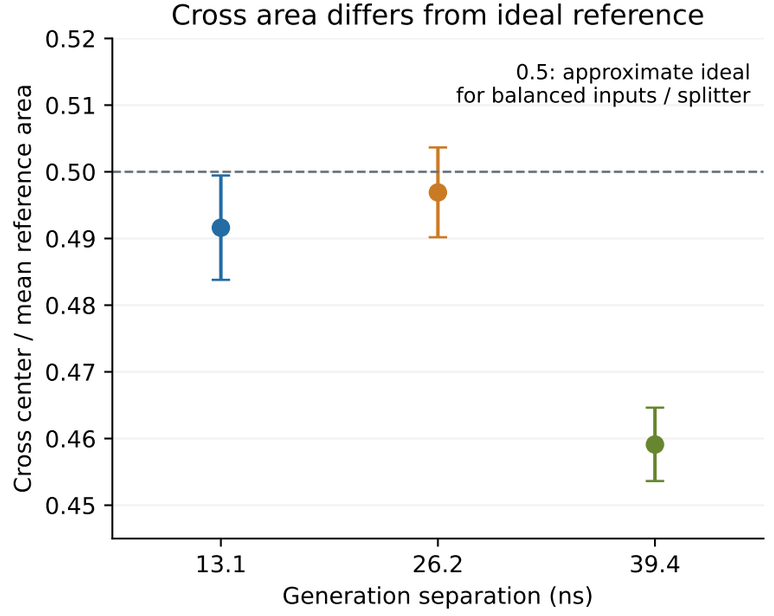

New side-peak-normalized analysis of Münzberg et al., Zenodo 6337697 (CC BY 4.0). No physical device measured by this project.
Error bars: 95% conditional Poisson count / shared calibration intervals; exclude normalization systematics. No microscopic defect or switching-rate inference.