A better control helps nominal inference; calibration ambiguity remains

Exploratory model selection → separately specified fresh validation. Original study and hardware circuits remain unchanged.

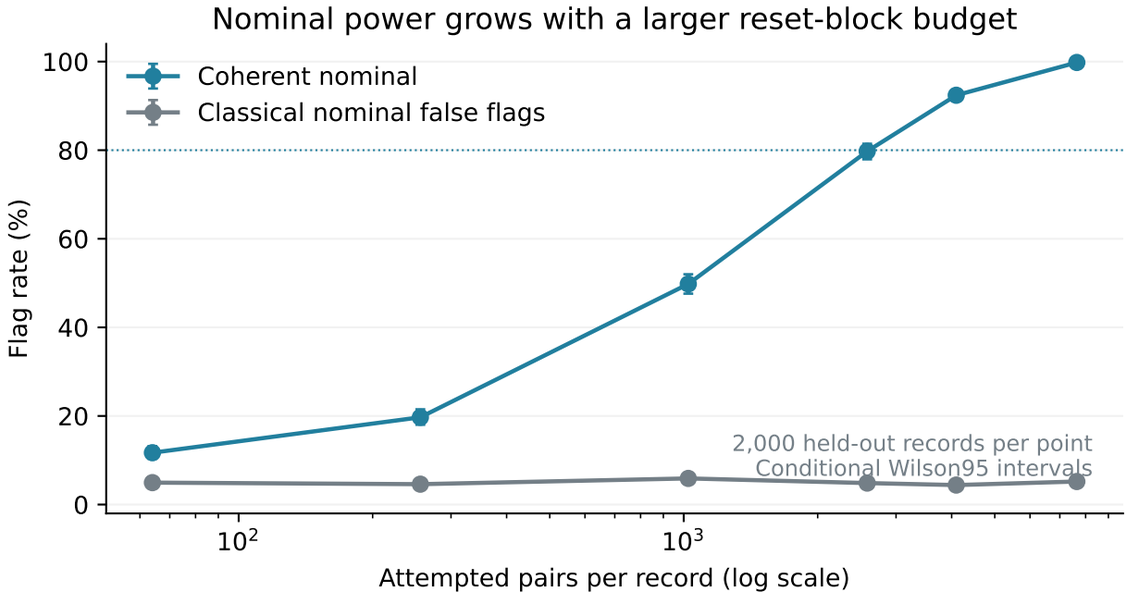

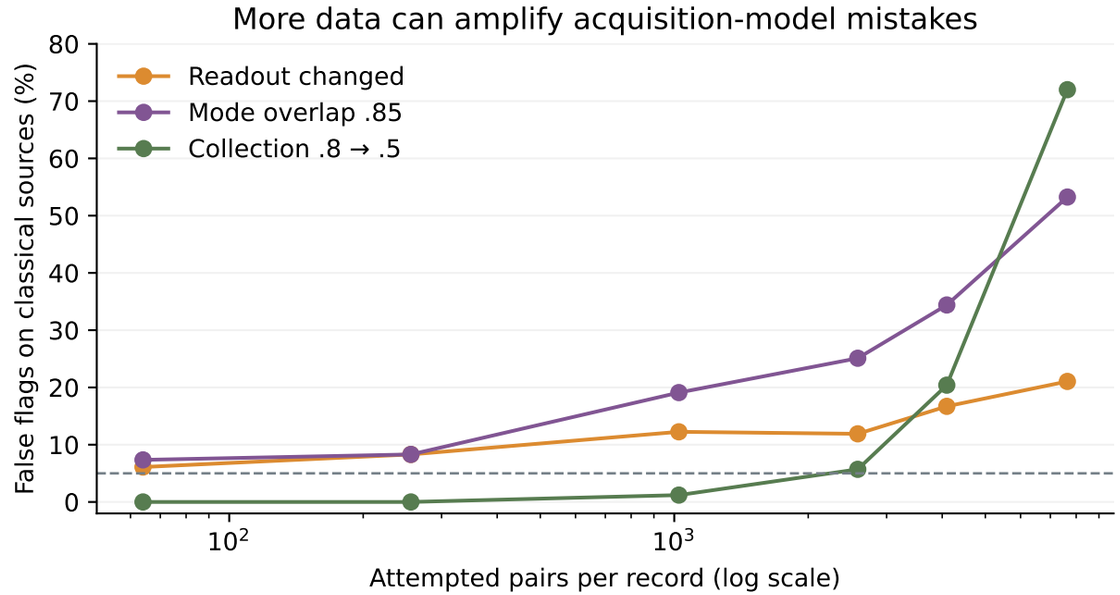

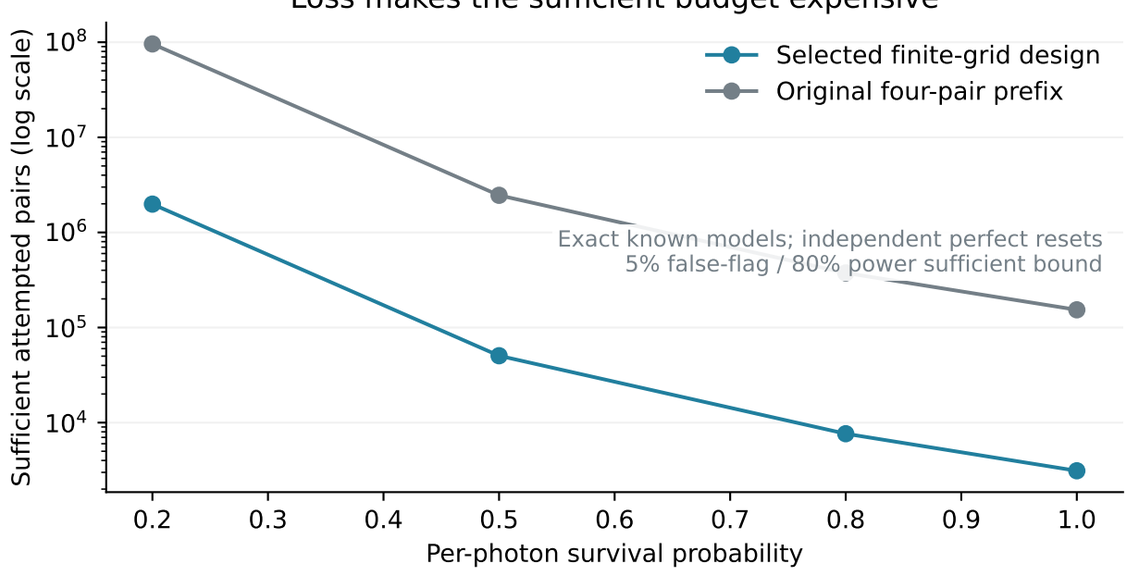

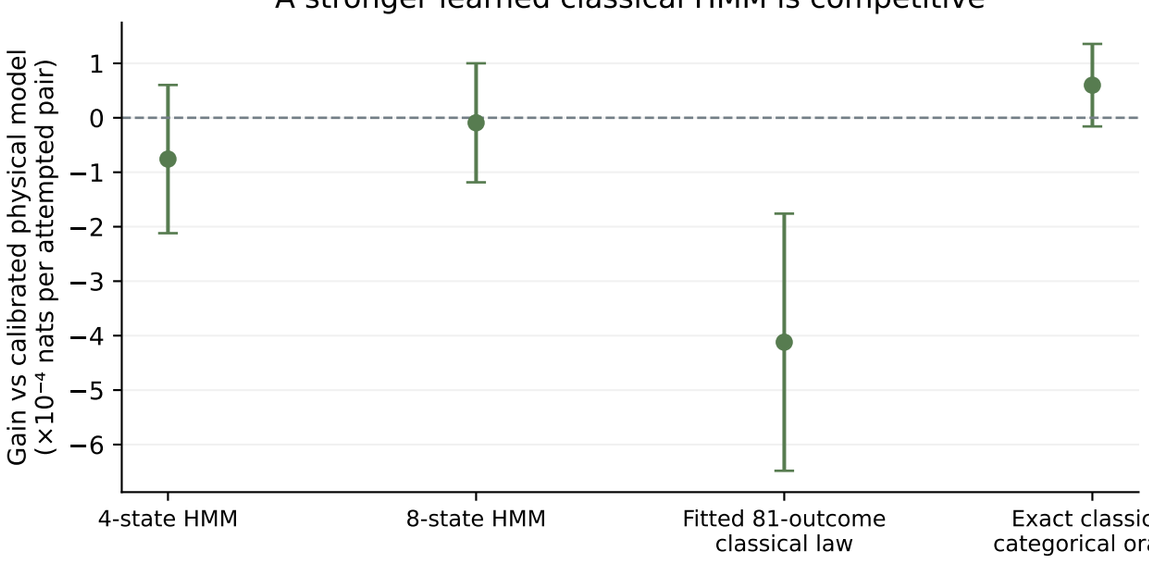

Synthetic four-pair blocks, with environment reset to I/2 between blocks. Reset fidelity/time and source-control feasibility are untested.
HMMs use the same 20,000 training blocks; physical predictors know source parameters. All 20 local EM starts hit the 200-iteration cap. No unique quantum-memory diagnosis.