A joint-photon instrument is implemented; useful diagnosis is not established

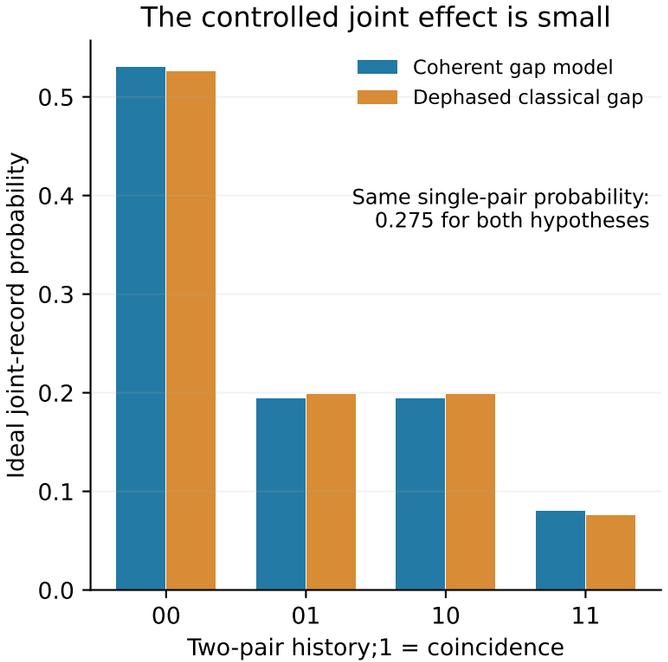

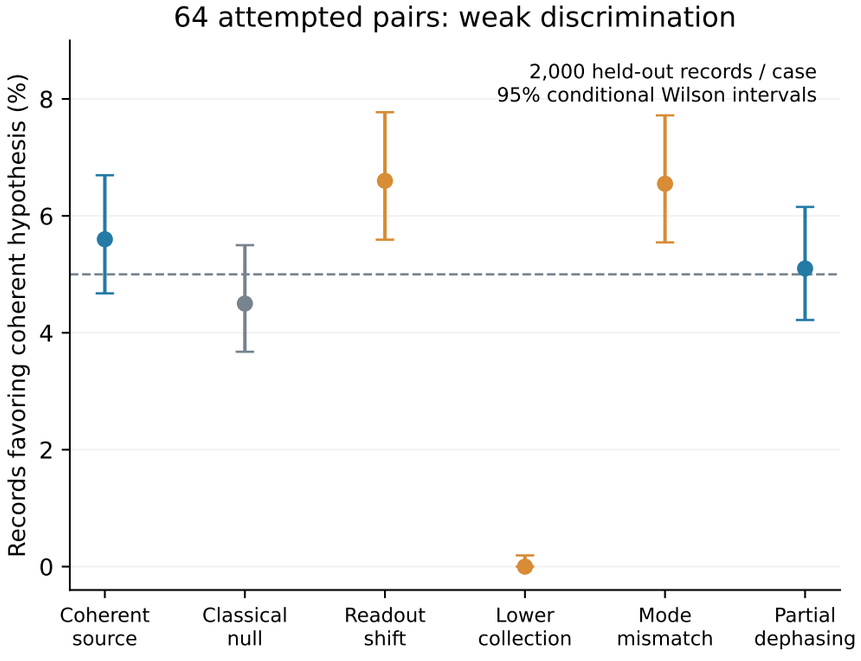

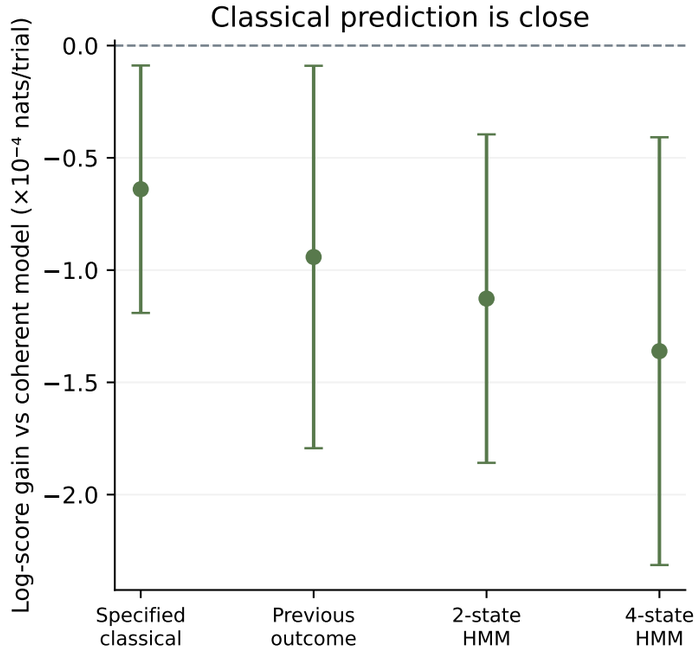

Passive measurement is exactly uninformative for these hypotheses. Controlled nominal flag rates:5.60% coherent versus4.50% classical null.
All data here are synthetic. Known physical parameters favor the specified model; HMMs learn from1,000 records. Intervals exclude model and calibration drift uncertainty.