

Date	Rabbit ID	BW (kg)	% BV removal	Group	Tele ID	EM info/Particle Conc			
5/4/23	AE M1 F013	1.5	45%	EM	8215	KC230503 bx1013	0.6 ml cet		
	pre-Anesthesia	End of Shock (+ min)	End of Res	1 H post Res	3H post Res	6H post Res	24H post Res	48H post Res	72H post Res
Lac (ABG/VBG)	1.4	3.8	4.0	1.8	3.8	2.5	1.6		
CBC (RBC/HGB/HCT) PLT	5.42 12	3.32 7.1	1.99 5.1	2.08 5.3	2.35 5.9	2.36 6	2.71 6.8		
	36.2	21	13.2	13.7	15.4	15.4	17.6		
	167	125	53	81	71	88	188		
CMP/TEG (when applicable)	✓✓	✓✓	✓✓	✓✓	✓✓	✓✓	✓✓		
HR	265	240	227	223	244	176	295		
MAP (Sys/Dia)	83	46	68	47	82	76	76		
	96/71	57/38	80/58	61/36	97/73	90/63	86/68		
Troponin Collection				✓		✓			
Time	6:35am	9:38	9:48	10:48	12:48pm	3:48pm	9:48a	9:48a	
Hemorrhage start time: 7:38am									
		Weight (kg)							

20% → 21 ml ✓
 15% → 45-75 ml ✓
 10% → 10-5 ml ✓
 in 1hr ✓

58
 @ 3H ✓
 @ 6H ✓
 @ 24H X

→ very active bunny ~~did not~~

ethanized
 ~ 11:30am
 5/5

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004

PATIENT REPORT

Syringe - S 65uL

06:55 AM

5/4/2023

Sample #

16917

Identifications

Patient ID

Patient last name

Patient first name

Sample type

T

Not specified
37.0 °C

BL

Blood gas values

pH

7.484

pCO₂

37.2

mmHg

pO₂

73.4

mmHg

Oximetry values

ctHb

10.3

g/dL

Hct_c

31.5

%

sO₂

97.2

%

FO₂Hb

95.8

%

FCOHb

2.4

%

FHHb

2.8

%

‡ FMetHb

< 0.0

%

Electrolyte values

cK⁺

4.2

meq/L

cNa⁺

142

meq/L

cCa²⁺

3.21

meq/L

cCl⁻

106

meq/L

Metabolite values

cGlu

141

mg/dL

cLac

1.4

mmol/L

Calculated values

cHCO₃⁻(P)_c

27.9

mmol/L

p50_e

23.75

mmHg

ABE_c

4.3

mmol/L

Notes

- ‡ Value(s) below the reportable range
- c Calculated value(s)
- e Estimated value(s)
- FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NQ-16

Printed

6:55:10AM

5/4/2023

Sensor cassette run #:

2588-190

RESULTS



ANIMAL NAME: Fo13_bl

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 5

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 922562

PLATE ID: 01980922562

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-03 10:29

MACHINE ID: 120007423

PRINT TIME: 2023-05-03 10:29

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	2.4g/dL	2.2-3.7			
TP	4.5g/dL	L 5.5-7.2			
GLOB	2.1g/dL	1.5-2.8			
A/G	1.17				
TB	0.1mg/dL	L 0.3-0.8			
GGT	9U/L	0-14			
AST	24U/L	0-98			
ALT	36U/L	31-53			
ALP	208U/L	H 70-145			
TBA	5.29umol/L				
AMY	199U/L	L 200-378			
LPS	140U/L				
LDH	160U/L	H 34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.6mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	9.93mg/dL	L 10.12-24.17			
BUN/CREA	65.392	21.000-236.000			
GLU	211.93mg/dL	H 75.14-145.24			
TC	50.40mg/dL	34.65-52.75			
TG	103.99mg/dL	26.10-153.12			
tCO2	36.4mmol/L	H 13.0-22.0			
Ca	12.18mg/dL	H 5.60-12.00			
PHOS	8.90mg/dL	H 1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

8617F4189

RESULTS



ANIMAL NAME: Fo13_bl

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 6

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-03 10:43

MACHINE ID: 120007423

PRINT TIME: 2023-05-03 10:43

Ver: V1.00.00.87/1.00.01.44


Assay	Result	Ref	Low	Normal	High
APTT	124.3s				
PT	15.8s				
TT	38.7s				
Fib	1.29g/L				

WAT: 2

EMP: 0

CHE: 0

4049E5028


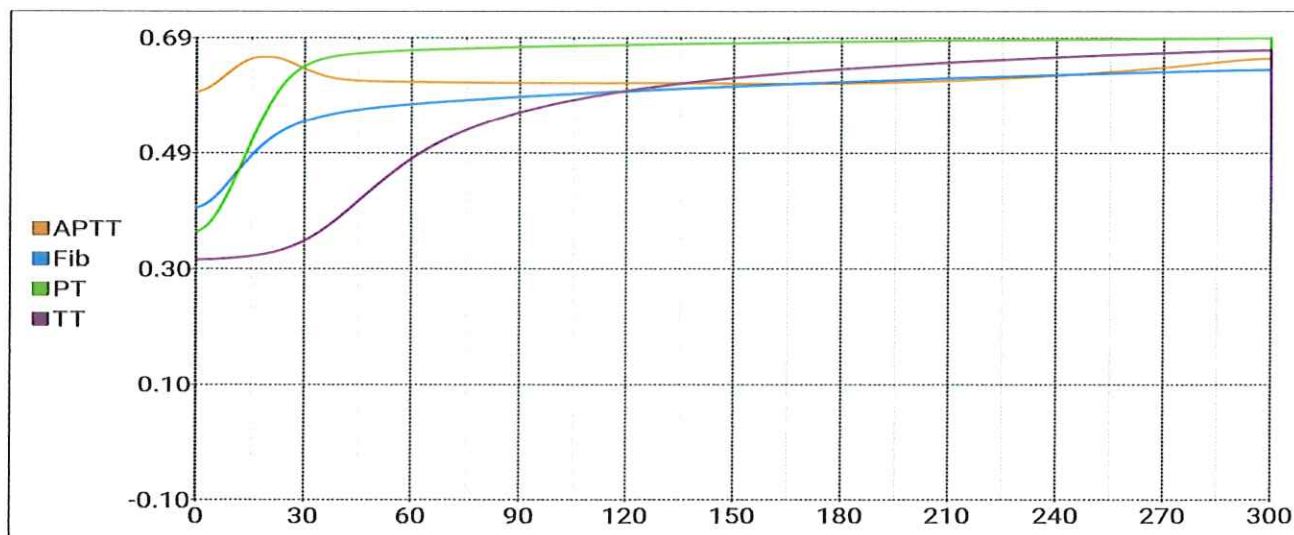


Note: The project curves from top to bottom are: APTT, Fib, PT, TT.

Patient Name :		Collect Date :	
Patient Number :		Operator : ABX	Department :
Seq.# : 20	Sample ID : 5	Physician :	
Birthdate :	Age :	Running Date : 05/03/2023 01:56:54 PM	Blood Type : Standard
Comment :			



				Range
WBC	4.6	10 ³ /mm ³		4.0 ... 10.0
	%	#		
NEU	1.0	!	0.05 IL	0.0 ... 99.9 2.00 ... 7.50
LYM	72.7		3.37	0.0 ... 99.9 1.00 ... 4.00
MON	3.0	!	0.14 IL	0.0 ... 99.9 0.20 ... 1.00
EOS	21.9		1.01 H	0.0 ... 99.9 0.00 ... 0.50
BAS	1.4		0.06	0.0 ... 99.9 0.00 ... 0.20

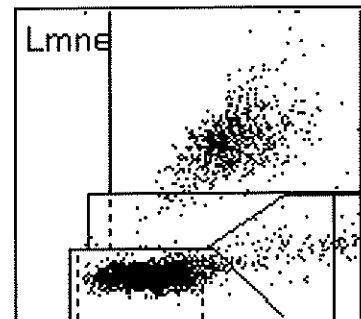

				Range
RBC	5.42	!	10 ⁶ /mm ³	3.80 ... 6.50
HGB	12.0		g/dl	11.5 ... 17.0
HCT	36.2	IL	%	37.0 ... 54.0
MCV	67	IL	μm ³	80 ... 100
MCH	22.2	L	pg	27.0 ... 32.0
MCHC	33.2		g/dl	32.0 ... 36.0
RDW	9.5	L	%	11.0 ... 16.0
PLT	167	!	10 ³ /mm ³	150 ... 500
MPV	5.5	L	μm ³	6.0 ... 11.0

Suspected Pathology
LEUKO : neutropenia, eosinophilia
ERYTHRO : microcytes, microcytosis

**Morphology Flags**

Leuko : RM
Erythro : MIC

Analyzer Alarms

WBC1	3406	WBC2	3490	LYM	2506	LL	0	FLN	7	WBC	3860
RBC1	21832	RBC2	21710	MON	105	ALY	53	FMN	2	RA#	3608
HCT1	1245193	HCT2	1239231	NEU	35	RM	41	FNE	4	DIF#	3389
PLT1	638	PLT2	641	EOS	743	LN	1	RN	0	CO%	96.97
HGBB	3510			NO	4	C127	79	LIC	106		
HGBM	2023										

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 09:05 AM 5/4/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16922

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type Not specified
 T 37.0 °C

EDS

Blood gas values

pH 7.446 [-]
 pCO₂ 42.1 mmHg [-]
 pO₂ 82.5 mmHg [-]

Oximetry values

ctHb 6.8 g/dL [-]
 Hct_c 21.0 %
 sO₂ 99.6 % [-]
 FO₂Hb 98.0 % [-]
 FCOHb 2.6 % [-]
 FHHb 0.4 % [-]
 ‡ FMetHb < 0.0 % [-]

Electrolyte values

cK⁺ 3.8 meq/L [-]
 cNa⁺ 139 meq/L [-]
 cCa²⁺ 2.82 meq/L [-]
 cCl⁻ 101 meq/L [-]

Metabolite values

cGlu 272 mg/dL [-]
 cLac 3.8 mmol/L [-]

Calculated values

cHCO₃⁻(P)_c 29.0 mmol/L
 p50_θ 24.78 mmHg
 ABE_c 4.5 mmol/L

Notes

‡ Value(s) below the reportable range
 c Calculated value(s)
 θ Estimated value(s)
 FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NQ-16 Sensor cassette run #: 2588-190
 Printed 9:06:07AM 5/4/2023

RESULTS

ANIMAL NAME:Fo13_eos

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:7

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:922757

PLATE ID:01980922757

OPERATOR ID:

LAB.:

TEST TIME:2023-05-04 10:48

MACHINE ID:120007423

PRINT TIME:2023-05-04 10:48

Ver:V1.00.00.87/1.00.01.44



Assay	Result	Ref	Low	Normal	High
ALB	1.8g/dL	L 2.2-3.7			
TP	3.0g/dL	L 5.5-7.2			
GLOB	1.2g/dL	L 1.5-2.8			
A/G	1.42				
TB	<0.1mg/dL	L 0.3-0.8			
GGT	4U/L	0-14			
AST	52U/L	0-98			
ALT	106U/L	H 31-53			
ALP	117U/L	70-145			
TBA	2.11umol/L				
AMY	166U/L	L 200-378			
LPS	53U/L				
LDH	109U/L	34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.6mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	15.32mg/dL	10.12-24.17			
BUN/CREA	101.640	21.000-236.000			
GLU	263.56mg/dL	H 75.14-145.24			
TC	60.23mg/dL	H 34.65-52.75			
TG	181.04mg/dL	H 26.10-153.12			
tCO2	22.9mmol/L	H 13.0-22.0			
Ca	9.34mg/dL	5.60-12.00			
PHOS	6.52mg/dL	H 1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

4799F1737

RESULTS

ANIMAL NAME: Fo13_eos

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 8

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-04 11:00

MACHINE ID: 120007423


PRINT TIME: 2023-05-04 11:00

Ver: V1.00.00.87/1.00.01.44



Assay	Result	Ref	Low	Normal	High
APTT	17.5s				
PT	15.0s				
TT	View curve				
Fib	3.63g/L				

The results are abnormal due to operation or other reasons, which need to be judged with the curve.

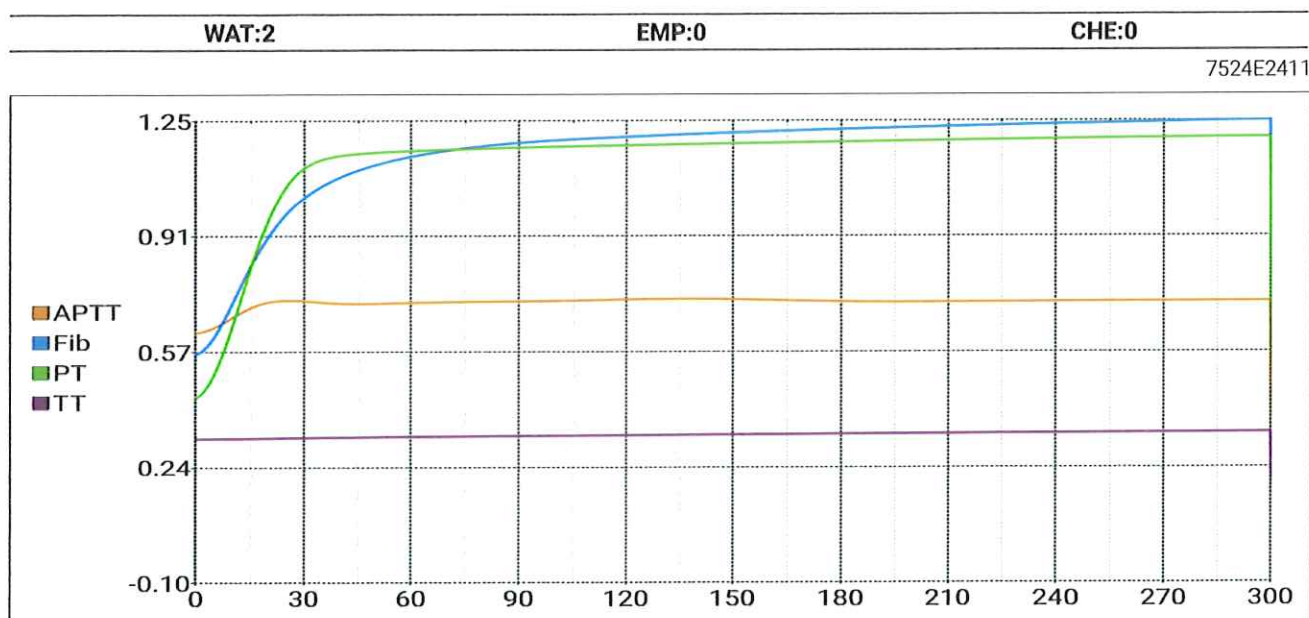

Note: The project curves from top to bottom are: APTT, Fib, PT, TT.

Patient Name :

Collect Date :

Patient Number :

Operator : ABX

Department :

Seq.# : 20

Sample ID : FD13-EOS

Physician :

Birthdate :

Age :

Gender :

Running Date : 05/04/2023 01:09:57 PM



Blood Type :

Standard

Comment :




				Range
WBC	7.2	10 ³ /mm ³		4.0 ... 10.0
	%	#		
NEU	---	---		0.0 ... 99.9 2.00 ... 7.50
LYM	71.2	5.11 H		0.0 ... 99.9 1.00 ... 4.00
MON	1.7	0.12 L		0.0 ... 99.9 0.20 ... 1.00
EOS	---	---		0.0 ... 99.9 0.00 ... 0.50
BAS	0.6	0.04		0.0 ... 99.9 0.00 ... 0.20

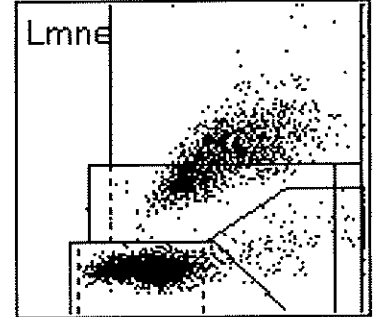

				Range
RBC	3.22	!L	10 ¹² /mm ³	3.80 ... 6.50
HGB	7.1	L	g/dl	11.5 ... 17.0
HCT	21.0	!L	%	37.0 ... 54.0
MCV	65	!L	μm ³	80 ... 100
MCH	22.0	L	pg	27.0 ... 32.0
MCHC	33.7		g/dl	32.0 ... 36.0
RDW	9.4	L	%	11.0 ... 16.0
PLT	125	!L	10 ³ /mm ³	150 ... 500
MPV	5.8	L	μm ³	6.0 ... 11.0

Suspected Pathology

LEUKO : lymphocytosis
ERYTHRO : anemia, microcytes, microcytosis



Morphology Flags

Leuko : NE
Erythro : MIC

Analyzer Alarms

WBC1	5324	WBC2	5216	LYM	3642	LL	1	FLN	1	WBC	5882
RBC1	13580	RBC2	13516	MON	88	ALY	35	FMN	1	RA#	5277
HCT1	762679	HCT2	763760	NEU	519	RM	12	FNE	85	DIF#	5080
PLT1	536	PLT2	517	EOS	831	LN	1	RN	0	CO%	98.01
HGBB	3511			NO	1	C127	79	LIC	91		
HGBM	2527										

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 09:17 AM 5/4/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16925

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type
 T Not specified
 37.0 °C

FOIR

Blood gas values

pH	7.370		[	-	]
pCO ₂	39.8	mmHg	[	-	]
pO ₂	97.8	mmHg	[	-	]

Oximetry values

cHb	4.6	g/dL	[	-	]
Hct _c	14.1	%			
§ sO ₂	> 100.0	%	[	-	]
FO ₂ Hb	98.0	%	[	-	]
FCOHb	2.5	%	[	-	]
§ FHHb	< 0.0	%	[	-	]
FMetHb	0.2	%	[	-	]

Electrolyte values

cK ⁺	3.6	meq/L	[	-	]
cNa ⁺	143	meq/L	[	-	]
cCa ²⁺	2.34	meq/L	[	-	]
cCl ⁻	105	meq/L	[	-	]

Metabolite values

cGlu	235	mg/dL	[	-	]
cLac	4.0	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	23.0	mmol/L
p50 _e	26.71	mmHg
ABE _c	-2.1	mmol/L

Notes

§ Value(s) above the reportable range
 § Value(s) below the reportable range
 c Calculated value(s)
 e Estimated value(s)
 FHHb 0094: Value below reportable range < 0.0
 sO₂ 0093: Value above reportable range > 100.0

Solution pack lot: NQ-16 Sensor cassette run #:
 Printed 9:17:28AM 5/4/2023 2588-190

RESULTS



ANIMAL NAME:Fo13_eor

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:11

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:922757

PLATE ID:01980922757

OPERATOR ID:

LAB.:

TEST TIME:2023-05-04 11:37

MACHINE ID:120007423

PRINT TIME:2023-05-04 11:37

Ver:V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	3.1g/dL	2.2-3.7			
TP	5.9g/dL	5.5-7.2			
GLOB	2.7g/dL	1.5-2.8			
A/G	1.13				
TB	<0.1mg/dL	L 0.3-0.8			
GGT	<2U/L	0-14			
AST	28U/L	0-98			
ALT	31U/L	31-53			
ALP	<5U/L	L 70-145			
TBA	<1.00umol/L				
AMY	86U/L	L 200-378			
LPS	41U/L				
LDH	70U/L	34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.3mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	16.16mg/dL	10.12-24.17			
BUN/CREA	191.135	21.000-236.000			
GLU	205.08mg/dL	H 75.14-145.24			
TC	151.96mg/dL	H 34.65-52.75			
TG	<26.10mg/dL	L 26.10-153.12			
tCO2	21.6mmol/L	13.0-22.0			
Ca	8.91mg/dL	5.60-12.00			
PHOS	12.37mg/dL	H 1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

385914J4629

RESULTS



ANIMAL NAME: Fo13_eor

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 12

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-04 11:52

MACHINE ID: 120007423

PRINT TIME: 2023-05-04 11:52

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
APTT	11.9s				
PT	24.2s				
TT	View curve				
Fib	1.89g/L				


The results are abnormal due to operation or other reasons, which need to be judged with the curve.

WAT:2

EMP:0

CHE:0

99747D5573

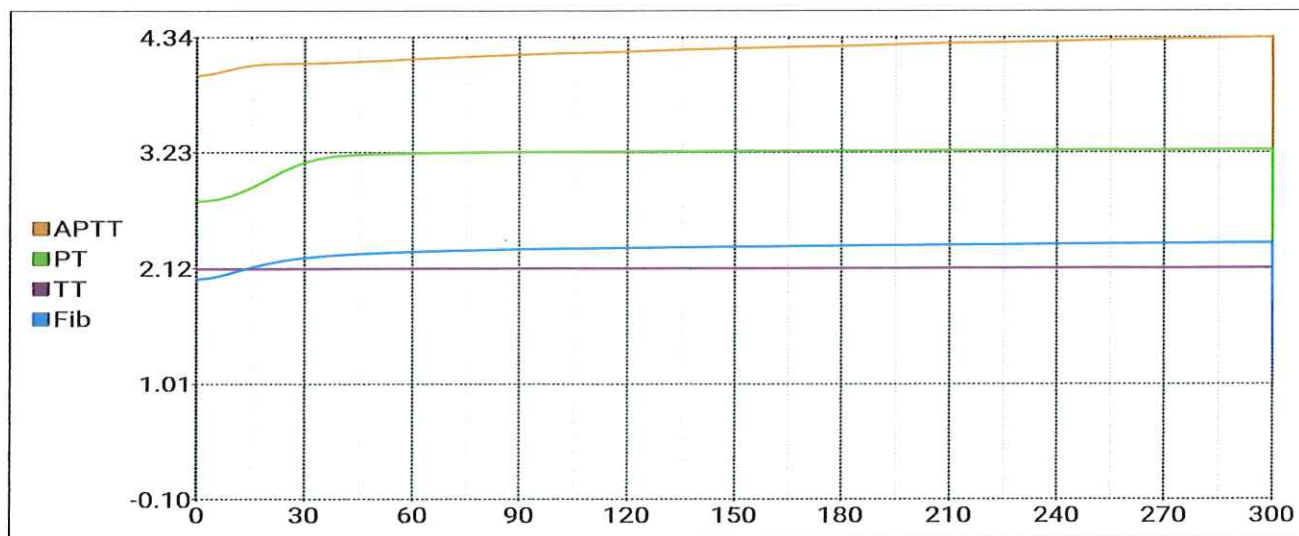



Note: The project curves from top to bottom are: APTT, PT, TT, Fib.

Patient Name :**Collect Date :****Patient Number :****Operator :** ABX**Department :****Seq.# :** 20**Sample ID :** FD13-EOR**Physician :****Birthdate :****Age :****Gender :****Running Date :** 05/04/2023 01:14:24 PM**Blood Type :**

Standard

Comment :

					Range
WBC	5.5	!	$10^3/\text{mm}^3$		4.0 ... 10.0
	%		#		
NEU	9.8	!	0.54	!L	0.0 ... 99.9 2.00 ... 7.50
LYM	87.2	!	4.83	!h	0.0 ... 99.9 1.00 ... 4.00
MON	1.0	!	0.06	!l	0.0 ... 99.9 0.20 ... 1.00
EOS	0.8	!	0.04	!	0.0 ... 99.9 0.00 ... 0.50
BAS	1.2	!	0.07	!	0.0 ... 99.9 0.00 ... 0.20

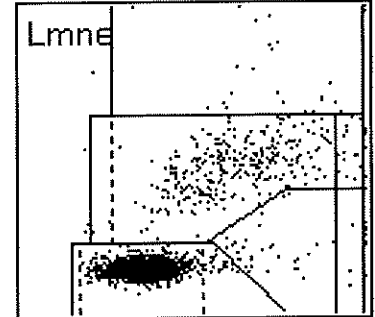

				Range
RBC	1.99	!L	$10^9/\text{mm}^3$	3.80 ... 6.50
HGB	5.1	L	g/dl	11.5 ... 17.0
HCT	13.2	!L	%	37.0 ... 54.0
MCV	66	!L	μm^3	80 ... 100
MCH	25.5	!	pg	27.0 ... 32.0
MCHC	38.5	H	g/dl	32.0 ... 36.0
RDW	9.7	L	%	11.0 ... 16.0
PLT	53	!L	$10^3/\text{mm}^3$	150 ... 500
MPV	6.0		μm^3	6.0 ... 11.0

**Suspected Pathology**

LEUKO : neutropenia
ERYTHRO : anemia, microcytes, microcytosis,
cold agglutinin
THROMBO : thrombopenia, platelet aggregats

Morphology Flags

Leuko : L1
Erythro : MIC

Analyzer Alarms

Analytic : LMNE-

WBC1	4133	WBC2	4076	LYM	2833	LL	1	FLN	2	WBC	3584
RBC1	8735	RBC2	8624	MON	33	ALY	20	FMN	0	RA#	3320
HCT1	497114	HCT2	494738	NEU	317	RM	3	FNE	7	DIF#	3209
PLT1	253	PLT2	236	EOS	26	LN	1	RN	13	CO%	97.95
HGBB	3510			NO	7	C127	20	LIC	36		
HGBM	2768										

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 10:20 AM 5/4/2023
PATIENT REPORT Syringe - S 65uL Sample # 16937

Identifications

Patient ID
Patient last name
Patient first name
Sample type Not specified
T 37.0 °C

11

Blood gas values

pH	7.471		[	-	]
pCO ₂	36.9	mmHg	[	-	]
pO ₂	95.4	mmHg	[	-	]

Oximetry values

cHb	4.8	g/dL	[	-	]
Hct _c	14.8	%			
‡ sO ₂	> 100.0	%	[	-	]
FO ₂ Hb	98.2	%	[	-	]
FCOHb	2.3	%	[	-	]
‡ FHHb	< 0.0	%	[	-	]
FMetHb	1.0	%	[	-	]

Electrolyte values

cK ⁺	3.5	meq/L	[	-	]
cNa ⁺	141	meq/L	[	-	]
cCa ²⁺	2.94	meq/L	[	-	]
cCl ⁻	103	meq/L	[	-	]

Metabolite values

cGlu	197	mg/dL	[	-	]
cLac	1.8	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	26.9	mmol/L
p50 _e	23.96	mmHg
ABE _c	2.9	mmol/L

Notes

‡ Value(s) above the reportable range
‡ Value(s) below the reportable range
c Calculated value(s)
e Estimated value(s)
FHHb 0094: Value below reportable range < 0.0
sO₂ 0093: Value above reportable range > 100.0

Solution pack lot: NQ-16 Sensor cassette run #: 2588-190
Printed 10:20:30AM 5/4/2023

RESULTS

ANIMAL NAME: Fo13_1h

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 17

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 922757

PLATE ID: 01980922757

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-04 12:57

MACHINE ID: 120007423

PRINT TIME: 2023-05-04 12:57

Ver: V1.00.00.87/1.00.01.44



Assay	Result	Ref	Low	Normal	High
ALB	3.0g/dL	2.2-3.7			
TP	5.7g/dL	5.5-7.2			
GLOB	2.7g/dL	1.5-2.8			
A/G	1.11				
TB	0.1mg/dL	L 0.3-0.8			
GGT	<2U/L	0-14			
AST	43U/L	0-98			
ALT	93U/L	H 31-53			
ALP	<5U/L	L 70-145			
TBA	<1.00umol/L				
AMY	102U/L	L 200-378			
LPS	38U/L				
LDH	124U/L	34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.7mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	16.68mg/dL	10.12-24.17			
BUN/CREA	92.462	21.000-236.000			
GLU	169.91mg/dL	H 75.14-145.24			
TC	181.97mg/dL	H 34.65-52.75			
TG	50.65mg/dL	26.10-153.12			
tCO2	22.9mmol/L	H 13.0-22.0			
Ca	10.38mg/dL	5.60-12.00			
PHOS	8.80mg/dL	H 1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

591314G9439

RESULTS

ANIMAL NAME: Fo13_1h

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 18

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-04 13:07

MACHINE ID: 120007423

PRINT TIME: 2023-05-04 13:08

Ver: V1.00.00.87/1.00.01.44




Assay	Result	Ref	Low	Normal	High
APTT	14.1s				
PT	17.0s				
TT	30.5s				
Fib	1.93g/L				

WAT:1

EMP:0

CHE:0

2135J0082

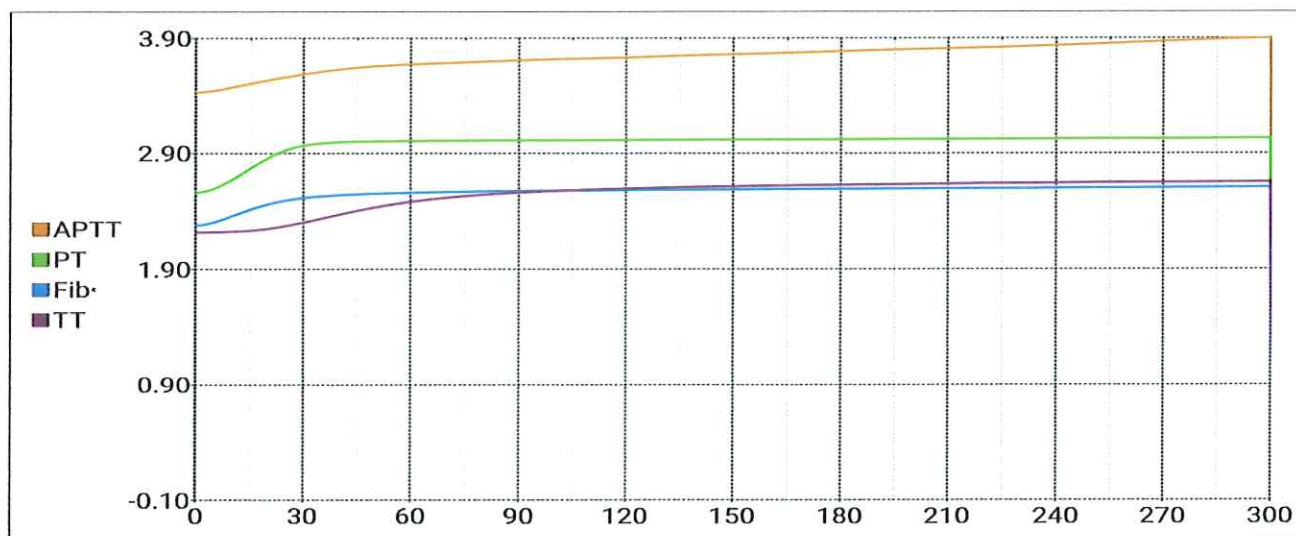

Note: The project curves from top to bottom are: APTT, PT, Fib, TT.

Patient Name :

Collect Date :

Patient Number :

Operator : ABX

Department :

Seq.# : 20

Sample ID : FD13-1hr

Physician :

Birthdate :

Age :


Gender :

Running Date : 05/04/2023 01:15:53 PM



Blood Type :

Standard

Comment :



		Range	
WBC	1.5 L	10 ³ /mm ³	4.0 ... 10.0
	%	#	
NEU	2.6	0.04 L	0.0 ... 99.9 2.00 ... 7.50
LYM	96.0	1.46	0.0 ... 99.9 1.00 ... 4.00
MON	0.6	0.01 I	0.0 ... 99.9 0.20 ... 1.00
EOS	0.4	0.01	0.0 ... 99.9 0.00 ... 0.50
BAS	0.4	0.01	0.0 ... 99.9 0.00 ... 0.20

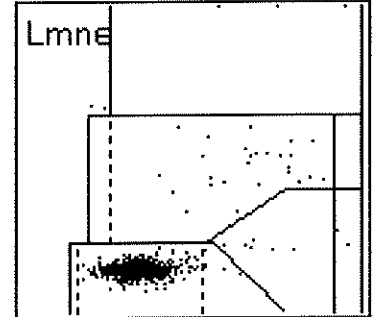

		Range	
RBC	2.08 !L	10 ⁹ /mm ³	3.80 ... 6.50
HGB	5.3 L	g/dl	11.5 ... 17.0
HCT	13.7 !L	%	37.0 ... 54.0
MCV	66 !L	μm ³	80 ... 100
MCH	25.7 I	pg	27.0 ... 32.0
MCHC	39.0 H	g/dl	32.0 ... 36.0
RDW	10.2 I	%	11.0 ... 16.0
PLT	81 !L	10 ³ /mm ³	150 ... 500
MPV	5.6 L	μm ³	6.0 ... 11.0

Suspected Pathology

LEUKO : leukopenia, neutropenia
ERYTHRO : anemia, microcytes, microcytosis,
cold agglutinin
THROMBO : thrombopenia
GEN. : pancytopenia



Morphology Flags

Erythro : MIC

Analyzer Alarms

WBC1	1137	WBC2	1163	LYM	1052	LL	0	FLN	1	WBC	1139
RBC1	8969	RBC2	9176	MON	7	ALY	2	FMN	0	RA#	1119
HCT1	508162	HCT2	521694	NEU	28	RM	1	FNE	1	DIF#	1091
PLT1	350	PLT2	342	EOS	4	LN	0	RN	0	CO%	97.76
HGBB	3512			NO	2	C127	0	LIC	1		
HGBM	2733										

RADIOMETER ABL90 SERIES

ABL90 1393-090R0199N0004 12:20 PM 5/4/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16953

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type
 T

Not specified
 37.0 °C

3H

Blood gas values

pH	7.519		[	-	]
pCO ₂	26.4	mmHg	[	-	]
pO ₂	86.7	mmHg	[	-	]

Oximetry values

cHb	5.3	g/dL	[	-	]
Hct _c	16.2	%			
‡ sO ₂	> 100.0	%	[	-	]
FO ₂ Hb	97.2	%	[	-	]
FCOHb	2.0	%	[	-	]
‡ FHHb	< 0.0	%	[	-	]
FMetHb	1.8	%	[	-	]

Electrolyte values

cK ⁺	3.8	meq/L	[	-	]
cNa ⁺	140	meq/L	[	-	]
cCa ²⁺	2.98	meq/L	[	-	]
cCl ⁻	106	meq/L	[	-	]

Metabolite values

cGlu	152	mg/dL	[	-	]
cLac	3.8	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	21.5	mmol/L
p50 _θ	22.38	mmHg
ABE _c	-1.4	mmol/L

Notes

‡ Value(s) above the reportable range
 ‡ Value(s) below the reportable range
 c Calculated value(s)
 θ Estimated value(s)
 FHHb 0094: Value below reportable range < 0.0
 sO₂ 0093: Value above reportable range > 100.0

Solution pack lot: NQ-16 Sensor cassette run #:
 Printed 12:20:56PM 5/4/2023 2588-190

RESULTS



ANIMAL NAME:Fo13_3h

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:25

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:922757

PLATE ID:01980922757

OPERATOR ID:

LAB.:

TEST TIME:2023-05-04 15:20

MACHINE ID:120007423

PRINT TIME:2023-05-04 15:21

Ver:V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	3.3g/dL	2.2-3.7			
TP	6.4g/dL	5.5-7.2			
GLOB	3.1g/dL	H 1.5-2.8			
A/G	1.07				
TB	0.1mg/dL	L 0.3-0.8			
GGT	<2U/L	0-14			
AST	56U/L	0-98			
ALT	48U/L	31-53			
ALP	<5U/L	L 70-145			
TBA	<1.00umol/L				
AMY	44U/L	L 200-378			
LPS	29U/L				
LDH	105U/L	34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.7mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	16.65mg/dL	10.12-24.17			
BUN/CREA	91.488	21.000-236.000			
GLU	130.30mg/dL	75.14-145.24			
TC	191.02mg/dL	H 34.65-52.75			
TG	161.66mg/dL	H 26.10-153.12			
tCO2	20.4mmol/L	13.0-22.0			
Ca	10.78mg/dL	5.60-12.00			
PHOS	7.33mg/dL	H 1.21-4.90			

CK> detection limit. Please dilute sample and re-test

* Abnormal sample: HEM? ICT? LIP?

WAT:0

EMP:0

CHE:0

096614A8064

RESULTS

ANIMAL NAME: Fo13_3

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 26

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-04 15:31

MACHINE ID: 120007423

PRINT TIME: 2023-05-04 15:31

Ver: V1.00.00.87/1.00.01.44




Assay	Result	Ref	Low	Normal	High
APTT	109.6s				
PT	18.1s				
TT	14.2s				
Fib	1.71g/L				

WAT:1

EMP:0

CHE:0

6926E8717

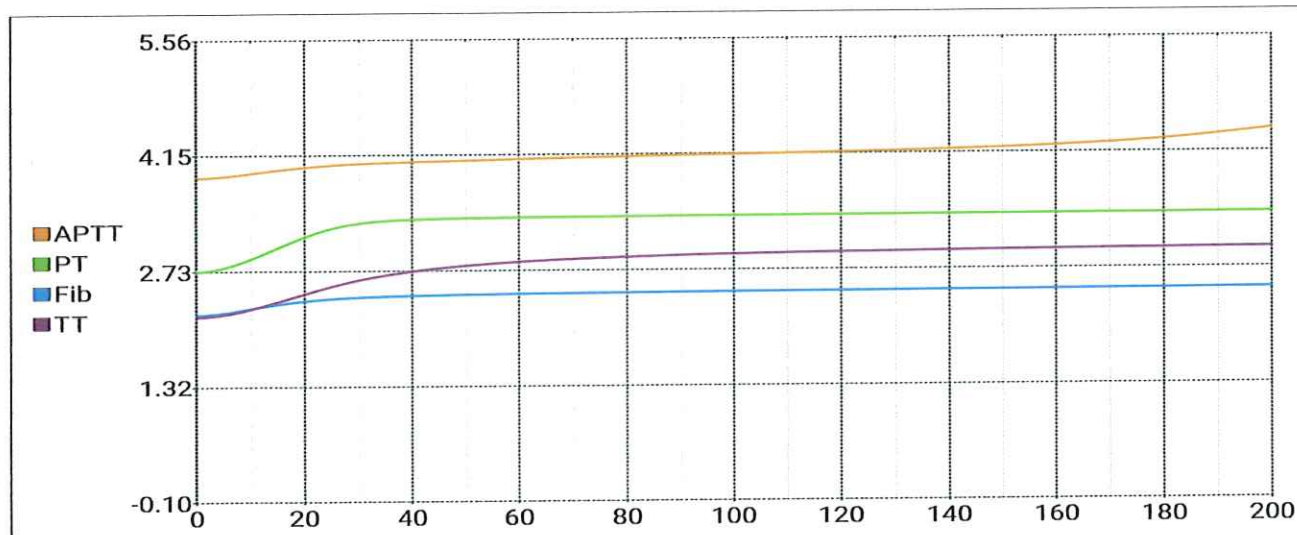


Note: The project curves from top to bottom are: APTT, PT, Fib, TT.

Patient Name :		Collect Date :	
Patient Number :		Operator : ABX	Department :
Seq.# : 20	Sample ID : FO13-3hr	Physician :	
Birthdate :	Age :	Running Date : 05/04/2023 02:23:32 PM	Blood Type : Standard
Comment :			




		Range	
WBC	1.0 L $10^3/\text{mm}^3$	4.0 ... 10.0	
	%	#	
NEU	3.7	0.04 L	0.0 ... 99.9 2.00 ... 7.50
LYM	92.2	0.94 L	0.0 ... 99.9 1.00 ... 4.00
MON	1.9	0.02 L	0.0 ... 99.9 0.20 ... 1.00
EOS	1.5	0.02	0.0 ... 99.9 0.00 ... 0.50
BAS	0.7	0.01	0.0 ... 99.9 0.00 ... 0.20



		Range	
RBC	2.35 IL $10^6/\text{mm}^3$	3.80 ... 6.50	
HGB	5.9 L g/dl	11.5 ... 17.0	
HCT	15.4 IL %	37.0 ... 54.0	
MCV	66 IL μm^3	80 ... 100	
MCH	25.2 I pg	27.0 ... 32.0	
MCHC	38.3 H g/dl	32.0 ... 36.0	
RDW	10.3 I %	11.0 ... 16.0	
PLT	71 IL $10^3/\text{mm}^3$	150 ... 500	
MPV	5.6 L μm^3	6.0 ... 11.0	

Suspected Pathology
LEUKO : leukopenia, lymphopenia, neutropenia
ERYTHRO : anemia, microcytes, microcytosis,
cold agglutinin
THROMBO : thrombopenia
GEN. : pancytopenia



Erythro : MIC

Morphology Flags

Analyzer Alarms

WBC1	758	WBC2	780	LYM	781	LL	1	FLN	1	WBC	895
RBC1	10185	RBC2	10110	MON	16	ALY	7	FMN	0	RA#	876
HCT1	576210	HCT2	572413	NEU	31	RM	2	FNE	1	DIF#	841
PLT1	310	PLT2	318	EOS	13	LN	0	RN	1	CO%	96.91
HGBB	3514			NO	0	C127	5	LIC	8		
HGBM	2663										

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 03:22 PM 5/4/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16957

Identifications

Patient ID

Patient last name

Patient first name

Sample type

Not specified

T

37.0 °C

bl

Blood gas values

pH	7.535		[	-	]
pCO ₂	24.6	mmHg	[	-	]
pO ₂	91.2	mmHg	[	-	]

Oximetry values

cHb	5.2	g/dL	[	-	]
Hct _c	15.9	%			
‡ sO ₂	> 100.0	%	[	-	]
FO ₂ Hb	96.3	%	[	-	]
FCOHb	2.2	%	[	-	]
‡ FHHb	< 0.0	%	[	-	]
FMetHb	3.2	%	[	-	]

Electrolyte values

cK ⁺	3.6	meq/L	[	-	]
cNa ⁺	141	meq/L	[	-	]
cCa ²⁺	2.67	meq/L	[	-	]
cCl ⁻	108	meq/L	[	-	]

Metabolite values

cGlu	148	mg/dL	[	-	]
cLac	2.5	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	20.7	mmol/L
p50 _e	21.64	mmHg
ABE _c	-1.9	mmol/L

Notes

‡ Value(s) above the reportable range
 ‡ Value(s) below the reportable range
 c Calculated value(s)
 e Estimated value(s)
 FHHb 0094: Value below reportable range < 0.0
 sO₂ 0093: Value above reportable range > 100.0

Solution pack lot: NQ-16

Printed 3:22:22PM 5/4/2023

Sensor cassette run #:

2588-190

RESULTS



ANIMAL NAME: Fo13_6h

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 27

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 922757

PLATE ID: 01980922757

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-04 16:09

MACHINE ID: 120007423

PRINT TIME: 2023-05-04 16:09

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	3.2g/dL	2.2-3.7			
TP	6.1g/dL	5.5-7.2			
GLOB	2.9g/dL	H 1.5-2.8			
A/G	1.10				
TB	0.2mg/dL	L 0.3-0.8			
GGT	<2U/L	0-14			
AST	85U/L	0-98			
ALT	53U/L	H 31-53			
ALP	<5U/L	L 70-145			
TBA	<1.00umol/L				
AMY	61U/L	L 200-378			
LPS	27U/L				
LDH	164U/L	H 34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.7mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	16.72mg/dL	10.12-24.17			
BUN/CREA	102.373	21.000-236.000			
GLU	136.69mg/dL	75.14-145.24			
TC	188.94mg/dL	H 34.65-52.75			
TG	86.05mg/dL	26.10-153.12			
tCO2	19.5mmol/L	13.0-22.0			
Ca	9.87mg/dL	5.60-12.00			
PHOS	6.86mg/dL	H 1.21-4.90			

CK> detection limit. Please dilute sample and re-test

* Abnormal sample: HEM? ICT? LIP?

WAT:0

EMP:0

CHE:0

071614A0966

RESULTS



ANIMAL NAME:Fo13_6h

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:28

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:9220185

PLATE ID:006509220185

OPERATOR ID:

LAB.:

TEST TIME:2023-05-04 16:35

MACHINE ID:120007423

PRINT TIME:2023-05-04 16:35

Ver:V1.00.00.87/1.00.01.44


Assay	Result	Ref	Low	Normal	High
APTT	8.4s				
PT	13.1s				
TT	47.2s				
Fib	1.79g/L				

WAT:1

EMP:0

CHE:0

85777H2532

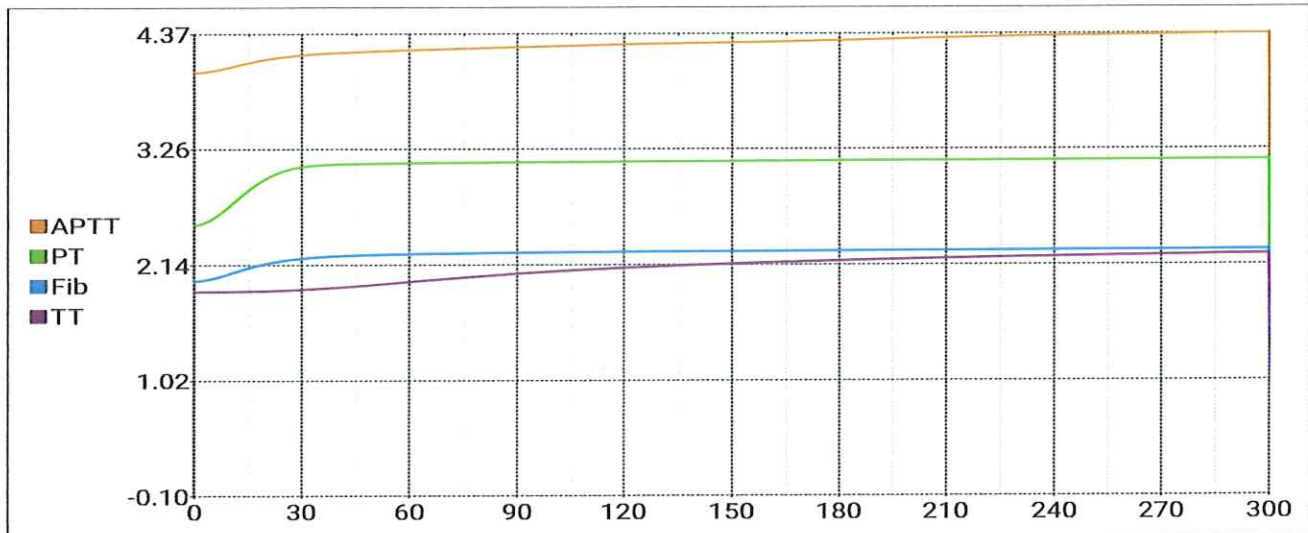

Note: The project curves from top to bottom are:APTT,PT,Fib,TT.

Patient Name :

Collect Date :

Patient Number :

Operator : ABX

Department :

Seq.# : 20

Sample ID : FO13-6h

Physician :

Birthdate :

Age :


Gender :

Running Date : 05/04/2023 05:34:57 PM Blood Type : Standard

Comment :



		Range	
WBC	1.5 L	10 ³ /mm ³	4.0 ... 10.0
	%	#	
NEU	27.5	0.40 L	0.0 ... 99.9 2.00 ... 7.50
LYM	62.3	0.91 L	0.0 ... 99.9 1.00 ... 4.00
MON	3.2	0.05 I	0.0 ... 99.9 0.20 ... 1.00
EOS	6.1	0.09	0.0 ... 99.9 0.00 ... 0.50
BAS	0.9	0.01	0.0 ... 99.9 0.00 ... 0.20

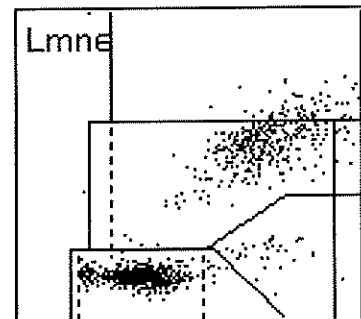

		Range	
RBC	2.36 !L	10 ⁶ /mm ³	3.80 ... 6.50
HGB	6.0 L	g/dl	11.5 ... 17.0
HCT	15.4 !L	%	37.0 ... 54.0
MCV	65 !L	µm ³	80 ... 100
MCH	25.3 I	pg	27.0 ... 32.0
MCHC	38.7 H	g/dl	32.0 ... 36.0
RDW	10.0 L	%	11.0 ... 16.0
PLT	88 !L	10 ³ /mm ³	150 ... 500
MPV	5.8 L	µm ³	6.0 ... 11.0



Suspected Pathology

LEUKO : leukopenia, lymphopenia, neutropenia
ERYTHRO : anemia, microcytes, microcytosis,
cold agglutinin
THROMBO : thrombopenia
GEN. : pancytopenia

Morphology Flags

Erythro : MIC

Analyzer Alarms

WBC1	1071	WBC2	1127	LYM	710	LL	16	FLN	1	WBC	1217
RBC1	10130	RBC2	10270	MON	37	ALY	7	FMN	0	RA#	1181
HCT1	569131	HCT2	577333	NEU	313	RM	1	FNE	17	DIF#	1129
PLT1	353	PLT2	395	EOS	69	LN	0	RN	6	CO%	97.45
HGBB	3513			NO	3	C127	12	LIC	19		
HGBM	2657										

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 09:20 AM 5/5/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16967

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type Not specified
 T 37.0 °C

24#

Blood gas values

pH	7.543		[	-	]
pCO ₂	32.8	mmHg	[	-	]
pO ₂	99.3	mmHg	[	-	]

Oximetry values

? ctHb	6.0	g/dL	[	-	]
? Hct _c	18.4	%			
? sO ₂	> 100.0	%	[	-	]
? FO ₂ Hb	97.1	%	[	-	]
? FCOHb	2.6	%	[	-	]
? FHHb	< 0.0	%	[	-	]
? FMetHb	2.6	%	[	-	]

Electrolyte values

cK ⁺	4.6	meq/L	[	-	]
cNa ⁺	145	meq/L	[	-	]
cCa ²⁺	2.79	meq/L	[	-	]
cCl ⁻	101	meq/L	[	-	]

Metabolite values

cGlu	147	mg/dL	[	-	]
cLac	1.6	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	28.2	mmol/L
? p50 _e	21.80	mmHg
? ABE _c	5.2	mmol/L

Notes




‡ Value(s) above the reportable range
 ‡ Value(s) below the reportable range
 c Calculated value(s)
 e Estimated value(s)
 ctHb 0581: OXI spectrum mismatch
 FCOHb 0581: OXI spectrum mismatch
 FHHb 0094: Value below reportable range < 0.0
 FHHb 0581: OXI spectrum mismatch
 FMetHb 0581: OXI spectrum mismatch
 FO₂Hb 0581: OXI spectrum mismatch
 sO₂ 0093: Value above reportable range > 100.0
 sO₂ 0581: OXI spectrum mismatch

Solution pack lot: NQ-16
 Printed 9:20:06AM 5/5/2023

Sensor cassette run #:
 2588-190

RESULT

Animal ID	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		
Sample ID FO13_24H	Analysis Date 05/05/2023 09:06:16	Operator JOY

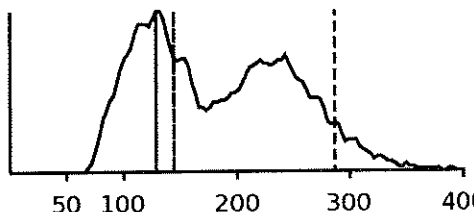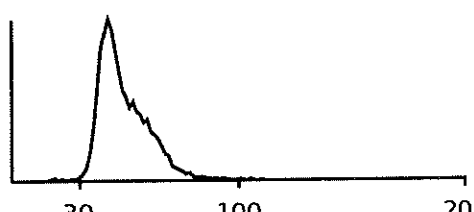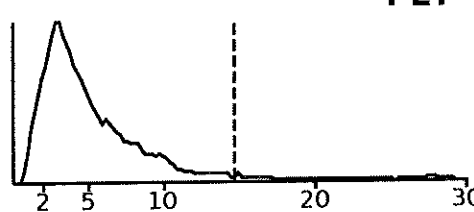Analyser Alarms			MIC, SCH, QCi, XB	
			Normal range	
WBC	5.0	$10^3/\text{mm}^3$	2.5	13.8
LYM%	---	%		
MON%	---	%		
GRA%	---	%		
(EOS%)	---	%		
LYM#	---	$10^3/\text{mm}^3$		
MON#	---	$10^3/\text{mm}^3$		
GRA#	---	$10^3/\text{mm}^3$		
EOS#	---	$10^3/\text{mm}^3$		
				
			WBC	
RBC	2.71	$10^6/\text{mm}^3$	4.80	7.20
HGB	6.8	g/dl	10.6	16.0
HCT	17.6	%	33.9	50.1
MCV	65	μm^3	62	79
MCH	25.1	pg	19.0	25.6
MCHC	38.6	g/dl	28.4	35.0
RDW	---	%		
				
			RBC	
PLT	188	$10^3/\text{mm}^3$	0	962
MPV	---	μm^3		
				
			PLT	

RESULTS



ANIMAL NAME: Fo13_24h

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 5

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 922757

PLATE ID: 01980922757

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-05 10:07

MACHINE ID: 120007423

PRINT TIME: 2023-05-05 10:07

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	3.3g/dL	2.2-3.7			
TP	6.2g/dL	5.5-7.2			
GLOB	3.0g/dL	H 1.5-2.8			
A/G	1.10				
TB	0.2mg/dL	L 0.3-0.8			
GGT	<2U/L	0-14			
AST	233U/L	H 0-98			
ALT	255U/L	H 31-53			
ALP	76U/L	70-145			
TBA	<1.00umol/L				
AMY	91U/L	L 200-378			
LPS	33U/L				
LDH	963U/L	H 34-129			
CK	> 4000U/L	H 218-2705			
Crea	<0.1mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	33.72mg/dL	H 10.12-24.17			
BUN/CREA	--	21.000-236.000			
GLU	135.65mg/dL	75.14-145.24			
TC	208.05mg/dL	H 34.65-52.75			
TG	196.46mg/dL	H 26.10-153.12			
tCO2	23.4mmol/L	H 13.0-22.0			
Ca	10.52mg/dL	5.60-12.00			
PHOS	9.62mg/dL	H 1.21-4.90			

-- means it can't be calculated.

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

972314E5674

RESULTS



ANIMAL NAME: Fo13_24

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 6

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-05-05 10:19

MACHINE ID: 120007423

PRINT TIME: 2023-05-05 10:19

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
APTT	9.6s				
PT	11.3s				
TT	View curve				
Fib	4.02g/L				


The results are abnormal due to operation or other reasons, which need to be judged with the curve.

WAT:0

EMP:0

CHE:0

6196D6383

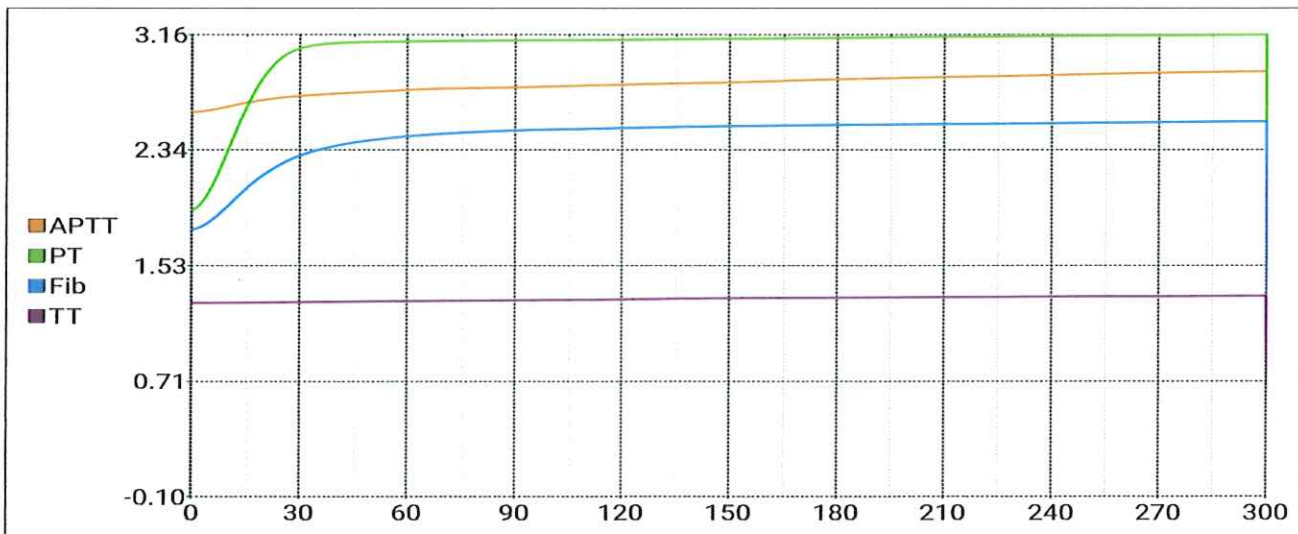

Note: The project curves from top to bottom are: APTT, PT, Fib, TT.