

Date	Rabbit ID	BW (Kg)	% BV removal	Group:				Tele ID	EM info/Particle Conc		
				10%	7.50%	5%	2.50%		24H Post Res	48H Post Res	
4/6/23	B-LR12	1.99	40%	remove + return in 10min every hour x 4				8215	—	—	0.80 ml ket
	pre-Anesthesia	End of Shock (+ min)	End of Res					End of Bleed	24H Post Res	48H Post Res	72H Post Res
Lac (ABG/VBG)	2.6	1.7	3.6	3.1	14.1	15	12.2	8.4	9.1	8.7	
CBC (RBC/HGB/HCT)	5.99	4.02	3.68					3.67	3.63	0.54	
	12.5	8.5	7.6					7.7	7.7	1.2	
	37.4	24.9	22.8					22.6	22.5	3.4	
PLT	304	279	252								
HR	260	227	234	168	283	293	205	199	298		
MAP (Sys/Dia)	104/71	64/39	58/35	56/37	62/37	80/53	77/47	80/48	88/57	79/62	
	85	49	45	47	47	64	57	63	71	64	
Coag Panel/ TEG	✓		✓				✓	✓	✓	✓	
CMP	✓		✓				✓	✓	✓	✓	
Troponin Collection							✓				
Time	0645	0902	912	1012	1112	1212	1312	1325	0912	0912	
Hemorrhage start time:			0702						Weight (kg)	1.99	

40
20 → 27.8
10 → 13.9
10 → 13.9

SWITCHED
FROM EM
TO LR (B)
DUE TO
VAP BUTTON
ISSUES.

BLOOD
COLLECTED
FROM VENOUS
PORT.

10 → 13.9
7.5 → 10.4
5.0 → 6.95
2.5 → 3.47

Excluded
low FDS Lac

RADIOMETER ABL90 SERIES

ABL90 1393-090R0199N0004

PATIENT REPORT

Syringe - S 65uL

06:26 AM

4/6/2023

Sample #

16380

Identifications

Patient ID

Patient last name

Patient first name

Sample type

T

Not specified

37.0 °C

Blood gas values

pH

7.457

pCO₂

41.1

mmHg

pO₂

74.3

mmHg

Oximetry values

? cHb

11.5

g/dL

? Hct_c

35.3

%

? sO₂

> 100.0

%

? FO₂Hb

> 100.0

%

? FCOHb

4.9

%

? FHHb

< 0.0

%

? FMetHb

< 0.0

%

Electrolyte values

cK⁺

4.4

meq/L

cNa⁺

142

meq/L

cCa²⁺

3.32

meq/L

cCl⁻

104

meq/L

Metabolite values

cGlu

136

mg/dL

cLac

2.6

mmol/L

Calculated values

cHCO₃⁻(P)_c

29.0

mmol/L

? p50_θ

23.79

mmHg

? ABE_c

4.7




mmol/L

Notes

- ‡ Value(s) above the reportable range
- ‡ Value(s) below the reportable range
- c Calculated value(s)
- θ Estimated value(s)
- cHb 0581: OXI spectrum mismatch
- FCOHb 0581: OXI spectrum mismatch
- FHHb 0094: Value below reportable range < 0.0
- FHHb 0581: OXI spectrum mismatch
- FMetHb 0094: Value below reportable range < 0.0
- FMetHb 0581: OXI spectrum mismatch
- FO₂Hb 0093: Value above reportable range > 100.0
- FO₂Hb 0581: OXI spectrum mismatch
- sO₂ 0093: Value above reportable range > 100.0
- sO₂ 0581: OXI spectrum mismatch

RESULT

Animal ID A_EM_GE05 8-121A	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		
Sample ID BASE	Analysis Date 04/06/2023 05:59:40	Operator MEB

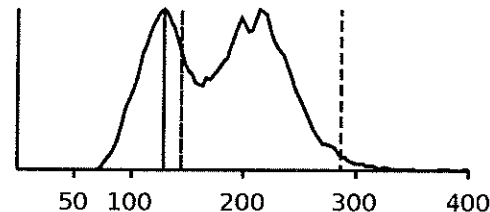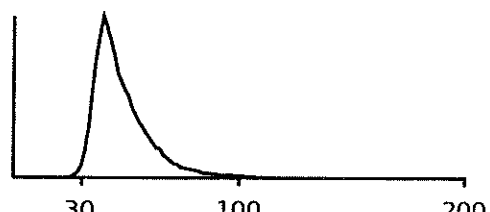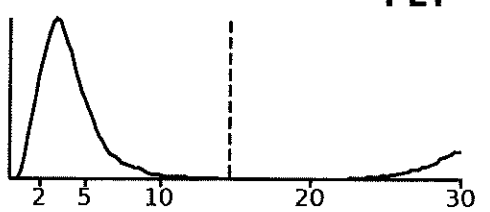Analyser Alarms Analysis Alarms				XB																																								
<table style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;"></th> <th style="text-align: left;"></th> <th style="text-align: left;"></th> <th style="text-align: left;">Normal range</th> </tr> </thead> <tbody> <tr> <td>WBC</td> <td>7.1</td> <td>$10^3/\text{mm}^3$</td> <td>2.5 13.8</td> </tr> <tr> <td>LYM%</td> <td>---</td> <td>%</td> <td></td> </tr> <tr> <td>MON%</td> <td>---</td> <td>%</td> <td></td> </tr> <tr> <td>GRA%</td> <td>---</td> <td>%</td> <td></td> </tr> <tr> <td>(EOS%)</td> <td>---</td> <td>%</td> <td></td> </tr> <tr> <td>LYM#</td> <td>---</td> <td>$10^3/\text{mm}^3$</td> <td></td> </tr> <tr> <td>MON#</td> <td>---</td> <td>$10^3/\text{mm}^3$</td> <td></td> </tr> <tr> <td>GRA#</td> <td>---</td> <td>$10^3/\text{mm}^3$</td> <td></td> </tr> <tr> <td>EOS#</td> <td>---</td> <td>$10^3/\text{mm}^3$</td> <td></td> </tr> </tbody> </table>							Normal range	WBC	7.1	$10^3/\text{mm}^3$	2.5 13.8	LYM%	---	%		MON%	---	%		GRA%	---	%		(EOS%)	---	%		LYM#	---	$10^3/\text{mm}^3$		MON#	---	$10^3/\text{mm}^3$		GRA#	---	$10^3/\text{mm}^3$		EOS#	---	$10^3/\text{mm}^3$		WBC 
			Normal range																																									
WBC	7.1	$10^3/\text{mm}^3$	2.5 13.8																																									
LYM%	---	%																																										
MON%	---	%																																										
GRA%	---	%																																										
(EOS%)	---	%																																										
LYM#	---	$10^3/\text{mm}^3$																																										
MON#	---	$10^3/\text{mm}^3$																																										
GRA#	---	$10^3/\text{mm}^3$																																										
EOS#	---	$10^3/\text{mm}^3$																																										
<table style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>RBC</td> <td>5.99</td> <td>$10^6/\text{mm}^3$</td> <td>4.80 7.20</td> </tr> <tr> <td>HGB</td> <td>12.5</td> <td>g/dl</td> <td>10.6 16.0</td> </tr> <tr> <td>HCT</td> <td>37.4</td> <td>%</td> <td>33.9 50.1</td> </tr> <tr> <td>MCV</td> <td>63</td> <td>μm^3</td> <td>62 79</td> </tr> <tr> <td>MCH</td> <td>20.9</td> <td>pg</td> <td>19.0 25.6</td> </tr> <tr> <td>MCHC</td> <td>33.5</td> <td>g/dl</td> <td>28.4 35.0</td> </tr> <tr> <td>RDW</td> <td>---</td> <td>%</td> <td></td> </tr> </tbody> </table>				RBC	5.99	$10^6/\text{mm}^3$	4.80 7.20	HGB	12.5	g/dl	10.6 16.0	HCT	37.4	%	33.9 50.1	MCV	63	μm^3	62 79	MCH	20.9	pg	19.0 25.6	MCHC	33.5	g/dl	28.4 35.0	RDW	---	%		RBC 												
RBC	5.99	$10^6/\text{mm}^3$	4.80 7.20																																									
HGB	12.5	g/dl	10.6 16.0																																									
HCT	37.4	%	33.9 50.1																																									
MCV	63	μm^3	62 79																																									
MCH	20.9	pg	19.0 25.6																																									
MCHC	33.5	g/dl	28.4 35.0																																									
RDW	---	%																																										
<table style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>PLT</td> <td>304</td> <td>$10^3/\text{mm}^3$</td> <td>0 962</td> </tr> <tr> <td>MPV</td> <td>---</td> <td>μm^3</td> <td></td> </tr> </tbody> </table>				PLT	304	$10^3/\text{mm}^3$	0 962	MPV	---	μm^3		PLT 																																
PLT	304	$10^3/\text{mm}^3$	0 962																																									
MPV	---	μm^3																																										

RESULTS

BH 1AANIMAL NAME: ~~Aemge5 base~~

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 1

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 922757

PLATE ID: 01980922757

OPERATOR ID:

LAB.:

TEST TIME: 2023-04-06 07:06

MACHINE ID: 120007423

PRINT TIME: 2023-04-06 07:06

Ver: V1.00.00.87/1.00.01.44



Assay	Result	Ref	Low	Normal	High
ALB	2.7g/dL	2.2-3.7			
TP	4.9g/dL	L 5.5-7.2			
GLOB	2.2g/dL	1.5-2.8			
A/G	1.19				
TB	<0.1mg/dL	L 0.3-0.8			
GGT	12U/L	0-14			
AST	43U/L	0-98			
ALT	57U/L	H 31-53			
ALP	110U/L	70-145			
TBA	5.87umol/L				
AMY	234U/L	200-378			
LPS	58U/L				
LDH	210U/L	H 34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.7mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	12.25mg/dL	10.12-24.17			
BUN/CREA	70.752	21.000-236.000			
GLU	149.41mg/dL	H 75.14-145.24			
TC	97.60mg/dL	H 34.65-52.75			
TG	185.43mg/dL	H 26.10-153.12			
tCO2	22.0mmol/L	H 13.0-22.0			
Ca	11.85mg/dL	5.60-12.00			
PHOS	4.56mg/dL	1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

6825F9218

RESULTS

BILLA BASEANIMAL NAME: ~~Acme05 base~~

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 2

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-04-06 07:17

MACHINE ID: 120007423

PRINT TIME: 2023-04-06 07:17

Ver: V1.00.00.87/1.00.01.44




Assay	Result	Ref	Low	Normal	High
APTT	139.1s				
PT	17.5s				
TT	42.9s				
Fib	2.85g/L				

WAT:0

EMP:0

CHE:0

3529F9878

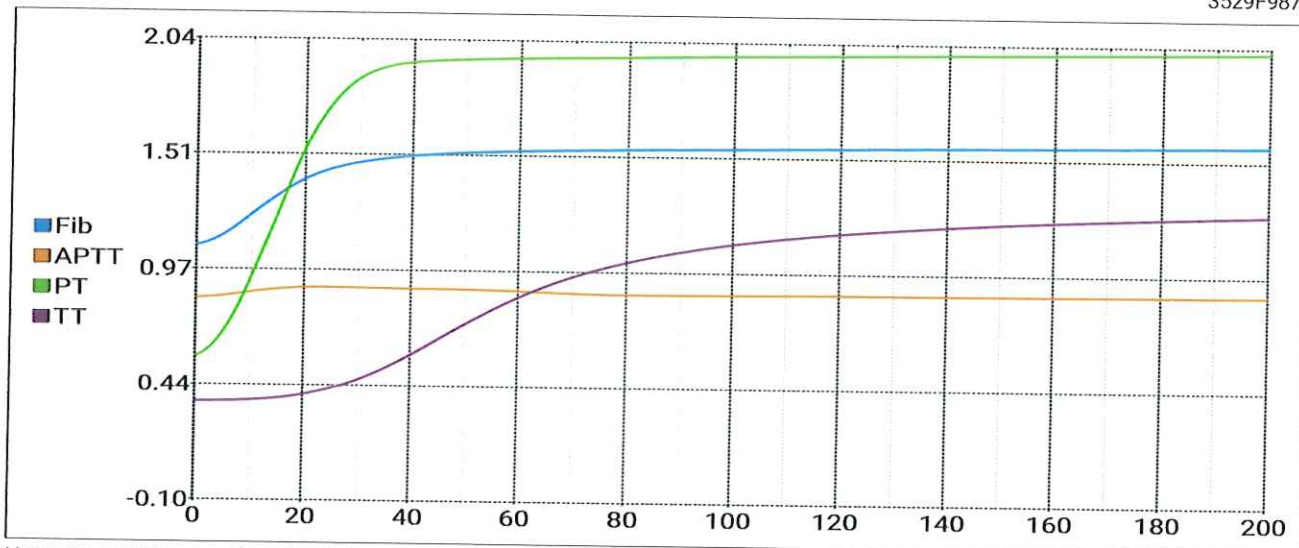

Note: The project curves from top to bottom are: Fib, APTT, PT, TT.

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004

08:43 AM

4/6/2023

PATIENT REPORT

Syringe - S 65uL

Sample #

16382

Identifications

Patient ID

Patient last name

Patient first name

Sample type

Not specified

T

37.0 °C

Blood gas values

pH 7.442 [-]

pCO₂ 52.2 mmHg [-]pO₂ 34.6 mmHg [-]

Oximetry values

ctHb 8.7 g/dL [-]

Hct_C 26.6 %sO₂ 61.3 % [-]FO₂Hb 59.6 % [-]

FCOHb 4.0 % [-]

FHHb 37.7 % [-]

‡ FMetHb < 0.0 % [-]

Electrolyte values

cK⁺ 3.4 meq/L [-]cNa⁺ 142 meq/L [-]cCa²⁺ 3.16 meq/L [-]cCl⁻ 99 meq/L [-]

Metabolite values

cGlu 200 mg/dL [-]

cLac 1.7 mmol/L [-]

Calculated values

cHCO₃⁻(P)_C 35.6 mmol/Lp50_e 29.06 mmHgABE_C 10.2 mmol/L

Notes

‡ Value(s) below the reportable range

c Calculated value(s)

e Estimated value(s)

FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NE-33

Sensor cassette run #: 2575-8


Printed 8:43:17AM 4/6/2023

RESULT


Animal ID B12LR	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		

Sample ID EOS	Analysis Date 04/06/2023 08:23:26	Operator MEB
-------------------------	---	------------------------

Analyser Alarms				XB
Analysis Alarms				

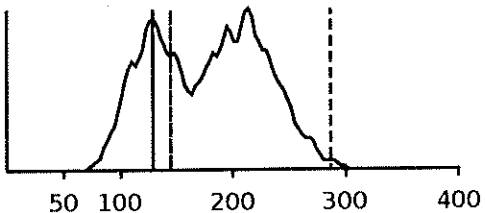WBC	3.7	10 ³ /mm ³	Normal range 2.5 13.8	
LYM%	---	%		WBC 
MON%	---	%		
GRA%	---	%		
(EOS%)	---	%		
LYM#	---	10 ³ /mm ³		
MON#	---	10 ³ /mm ³		
GRA#	---	10 ³ /mm ³		
EOS#	---	10 ³ /mm ³		

RBC	4.02	L 10 ⁶ /mm ³	4.80 7.20	
HGB	8.5	L g/dl	10.6 16.0	RBC 
HCT	24.9	L %	33.9 50.1	
MCV	62	μm ³	62 79	
MCH	21.1	pg	19.0 25.6	
MCHC	34.0	g/dl	28.4 35.0	
RDW	---	%		

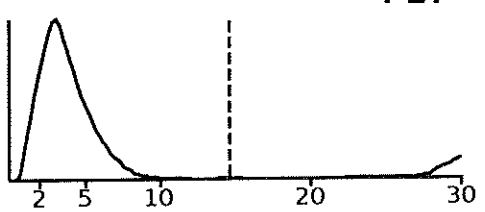PLT	279	10 ³ /mm ³	0 962	
MPV	---	μm ³		PLT 

RADIOMETER ABL90 SERIES

ABL90 1393-090R0199N0004
 PATIENT REPORT Syringe - S 65uL 08:59 AM 4/6/2023
 Sample # 16383

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type T Not specified
 37.0 °C

Blood gas values

pH	7.472		[	-	]
pCO ₂	46.3	mmHg	[	-	]
pO ₂	31.9	mmHg	[	-	]

Oximetry values

ctHb	7.5	g/dL	[	-	]
Hct _c	23.1	%			
sO ₂	56.3	%	[	-	]
FO ₂ Hb	54.8	%	[	-	]
FCOHb	3.7	%	[	-	]
FHHb	42.6	%	[	-	]
‡ FMetHb	< 0.0	%	[	-	]

Electrolyte values

cK ⁺	3.4	meq/L	[	-	]
cNa ⁺	141	meq/L	[	-	]
cCa ²⁺	3.09	meq/L	[	-	]
cCl ⁻	100	meq/L	[	-	]

Metabolite values

cGlu	190	mg/dL	[	-	]
cLac	3.6	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	33.8	mmol/L
p50 _e	28.90	mmHg
ABE _c	9.2	mmol/L

Notes




‡ Value(s) below the reportable range
 c Calculated value(s)
 e Estimated value(s)
 FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NE-33
 Printed 8:59:06AM 4/6/2023

Sensor cassette run #: 2575-8

RESULT

Animal ID B12LR	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		
Sample ID EOR	Analysis Date 04/06/2023 08:36:28	Operator MEB

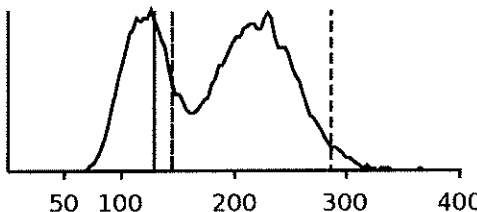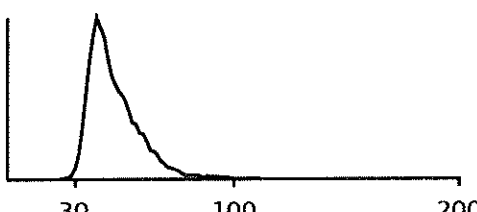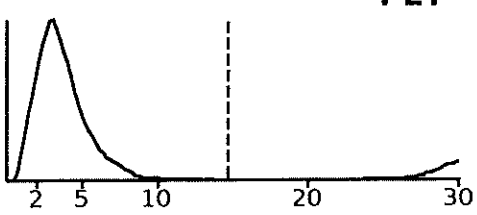Analyser Alarms			Analysis Alarms		XB	
			Normal range			
WBC	4.6	10 ³ /mm ³	2.5	13.8		
LYM%	---	%				
MON%	---	%				
GRA%	---	%				
(EOS%)	---	%				
LYM#	---	10 ³ /mm ³				
MON#	---	10 ³ /mm ³				
GRA#	---	10 ³ /mm ³				
EOS#	---	10 ³ /mm ³				
						
			WBC			
RBC	3.68	L 10 ⁶ /mm ³	4.80	7.20		
HGB	7.6	L g/dl	10.6	16.0		
HCT	22.8	L %	33.9	50.1		
MCV	62	μm ³	62	79		
MCH	20.6	pg	19.0	25.6		
MCHC	33.3	g/dl	28.4	35.0		
RDW	---	%				
						
			RBC			
PLT	252	10 ³ /mm ³	0	962		
MPV	---	μm ³				
						
			PLT			

RESULTS



ANIMAL NAME: B12lr eor

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 5

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 922757

PLATE ID: 01980922757

OPERATOR ID:

LAB.:

TEST TIME: 2023-04-06 09:45

MACHINE ID: 120007423

PRINT TIME: 2023-04-06 09:45

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	1.6g/dL	L 2.2-3.7			
TP	3.2g/dL	L 5.5-7.2			
GLOB	1.6g/dL	1.5-2.8			
A/G	1.01				
TB	<0.1mg/dL	L 0.3-0.8			
GGT	4U/L	0-14			
AST	28U/L	0-98			
ALT	35U/L	31-53			
ALP	68U/L	L 70-145			
TBA	<1.00umol/L				
AMY	138U/L	L 200-378			
LPS	84U/L				
LDH	275U/L	H 34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.7mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	12.87mg/dL	10.12-24.17			
BUN/CREA	71.476	21.000-236.000			
GLU	189.90mg/dL	H 75.14-145.24			
TC	67.16mg/dL	H 34.65-52.75			
TG	267.79mg/dL	H 26.10-153.12			
tCO2	26.9mmol/L	H 13.0-22.0			
Ca	10.14mg/dL	5.60-12.00			
PHOS	4.78mg/dL	1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

7063F8742

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 09:41 AM 4/6/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16385

Identifications

Patient ID
 Patient last name 10%
 Patient first name REMOVE/RETURN
 Sample type Not specified
 T 37.0 °C

Blood gas values

pH 7.489 [-]
 pCO₂ 45.4 mmHg [-]
 pO₂ 33.0 mmHg [-]

Oximetry values

cHb 7.8 g/dL [-]
 Hct_C 23.9 %
 sO₂ 60.7 % [-]
 FO₂Hb 59.1 % [-]
 FCOHb 3.8 % [-]
 FHHb 38.3 % [-]
 ‡ FMetHb < 0.0 % [-]

Electrolyte values

cK⁺ 3.0 meq/L [-]
 cNa⁺ 142 meq/L [-]
 cCa²⁺ 3.07 meq/L [-]
 cCl⁻ 99 meq/L [-]

Metabolite values

cGlu 214 mg/dL [-]
 cLac 3.1 mmol/L [-]

Calculated values

cHCO₃⁻(P)_C 34.5 mmol/L
 p50_θ 27.95 mmHg
 ABE_C 10.2 mmol/L

Notes

‡ Value(s) below the reportable range
 c Calculated value(s)
 θ Estimated value(s)
 FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NE-33 Sensor cassette run #: 2575-8
 Printed 9:41:14AM 4/6/2023

RADIOMETER ABL90 SERIES

ABL90 1393-090R0199N0004 10:46 AM 4/6/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16390

Identifications

Patient ID 7.5%
 Patient last name REMOVE/RETURN
 Patient first name
 Sample type Not specified
 T 37.0 °C

Blood gas values

pH 7.224 [-]
 pCO₂ 54.6 mmHg [-]
 pO₂ 22.4 mmHg [-]

Oximetry values

cHb 7.5 g/dL [-]
 Hct_c 22.9 %
 sO₂ 19.0 % [-]
 FO₂Hb 18.4 % [-]
 FCOHb 2.2 % [-]
 FHHb 78.7 % [-]
 FMetHb 0.7 % [-]

Electrolyte values

cK⁺ 2.9 meq/L [-]
 cNa⁺ 141 meq/L [-]
 cCa²⁺ 2.82 meq/L [-]
 cCl⁻ 97 meq/L [-]

Metabolite values

? cGlu > 270 mg/dL [-]
 cLac 14.1 mmol/L [-]

Calculated values

cHCO₃⁻(P)_c 22.6 mmol/L
 p50_c 40.17 mmHg
 ABE_c -4.9 mmol/L

Notes

c Calculated value(s)
 cGlu 1402: pO2 too low. cGlucose Linearity out of range.

Solution pack lot: NE-33
 Printed 10:46:03AM 4/6/2023

Sensor cassette run #: 2575-8

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 11:44 AM 4/6/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16393

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type Not specified
 T 37.0 °C

5%
 REMOVE/RETURN

Blood gas values

pH	7.295		[-]
pCO ₂	38.7	mmHg	[-]
pO ₂	31.9	mmHg	[-]

Oximetry values

ctHb	7.6	g/dL	[-]
Hct _C	23.2	%	
sO ₂	43.1	%	[-]
FO ₂ Hb	42.0	%	[-]
FCOHb	3.1	%	[-]
FHHb	55.5	%	[-]
‡ FMetHb	< 0.0	%	[-]

Electrolyte values

cK ⁺	2.9	meq/L	[-]
cNa ⁺	142	meq/L	[-]
cCa ⁺⁺	2.73	meq/L	[-]
cCl ⁻	101	meq/L	[-]

Metabolite values

cGlu	357	mg/dL	[-]
cLac	15	mmol/L	[-]

Calculated values

cHCO ₃ ⁻ (P) _C	18.8	mmol/L
p50 _θ	35.50	mmHg
ABE _C	-7.1	mmol/L

Notes

‡ Value(s) below the reportable range
 c Calculated value(s)
 θ Estimated value(s)
 FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NE-33 Sensor cassette run #: 2575-8
 Printed 11:45:01AM 4/6/2023

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 12:30 PM 4/6/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16395

Identifications

Patient ID 2.5 %
 Patient last name REMOVE/RETURN
 Patient first name
 Sample type Not specified
 T 37.0 °C

Blood gas values

pH	7.417		[	-	]
pCO ₂	37.0	mmHg	[	-	]
pO ₂	31.1	mmHg	[	-	]

Oximetry values

ctHb	7.6	g/dL	[	-	]
Hct _c	23.2	%			
sO ₂	49.9	%	[	-	]
FO ₂ Hb	48.6	%	[	-	]
FCOHb	3.4	%	[	-	]
FHHb	48.8	%	[	-	]
‡ FMetHb	< 0.0	%	[	-	]

Electrolyte values

cK ⁺	3.0	meq/L	[	-	]
cNa ⁺	142	meq/L	[	-	]
cCa ²⁺	2.98	meq/L	[	-	]
cCl ⁻	99	meq/L	[	-	]

Metabolite values

cGlu	317	mg/dL	[	-	]
cLac	12.2	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	23.8	mmol/L
p50 _θ	31.14	mmHg
ABE _c	-0.6	mmol/L

Notes

‡ Value(s) below the reportable range
 c Calculated value(s)
 θ Estimated value(s)
 FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NE-33 Sensor cassette run #: 2575-8
 Printed 12:30:36PM 4/6/2023

RADIOMETER ABL90 SERIES

ABL90 1393-090R0199N0004 01:12 PM 4/6/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16398

Identifications

Patient ID

Patient last name

Patient first name

Sample type

T

Not specified

37.0 °C

EOB

~~24.6 %~~

~~REMOVE FROM VIEW~~

Blood gas values

pH	7.425		[	-	]
pCO ₂	37.8	mmHg	[	-	]
pO ₂	33.9	mmHg	[	-	]

Oximetry values

ctHb	7.5	g/dL	[	-	]
Hct _C	23.0	%			
sO ₂	56.6	%	[	-	]
FO ₂ Hb	55.1	%	[	-	]
FCOHb	3.6	%	[	-	]
FHHb	42.2	%	[	-	]
‡ FMetHb	< 0.0	%	[	-	]

Electrolyte values

cK ⁺	2.9	meq/L	[	-	]
cNa ⁺	143	meq/L	[	-	]
cCa ²⁺	2.99	meq/L	[	-	]
cCl ⁻	103	meq/L	[	-	]

Metabolite values

cGlu	246	mg/dL	[	-	]
cLac	8.4	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _C	24.8	mmol/L
p50 _θ	30.67	mmHg
ABE _C	0.4	mmol/L

Notes

‡ Value(s) below the reportable range
 c Calculated value(s)
 θ Estimated value(s)
 FMetHb 0094: Value below reportable range < 0.0

Solution pack lot: NE-33
 Printed 1:12:27PM 4/6/2023


Sensor cassette run #: 2575-8

RESULT


Animal ID B12LR	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		
Sample ID EOB	Analysis Date 04/06/2023 12:52:23	Operator JOY

Analyser Alarms Analysis Alarms	XB
--	----


WBC	4.6	$10^3/\text{mm}^3$	Normal range 2.5 13.8	
LYM%	--,--	%		
MON%	--,--	%		
GRA%	--,--	%		
(EOS%)	--,--	%		
LYM#	--,--	$10^3/\text{mm}^3$		
MON#	--,--	$10^3/\text{mm}^3$		
GRA#	--,--	$10^3/\text{mm}^3$		
EOS#	--,--	$10^3/\text{mm}^3$		

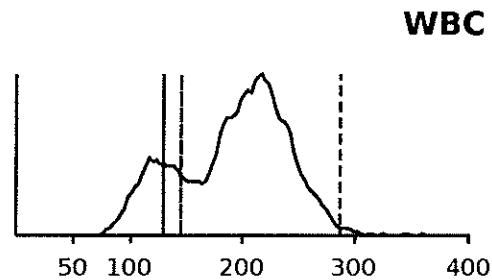

RBC	3.67	L $10^6/\text{mm}^3$	4.80 7.20	
HGB	7.7	L g/dl	10.6 16.0	
HCT	22.6	L %	33.9 50.1	
MCV	61	L μm^3	62 79	
MCH	21.0	pg	19.0 25.6	
MCHC	34.2	g/dl	28.4 35.0	
RDW	--,--	%		

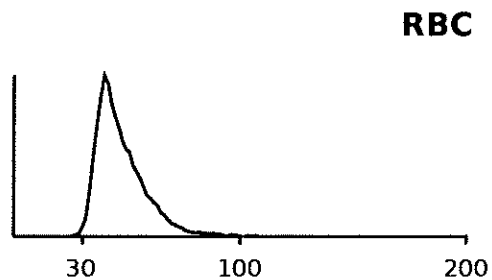

PLT	295	$10^3/\text{mm}^3$	0 962	
MPV	--,--	μm^3		

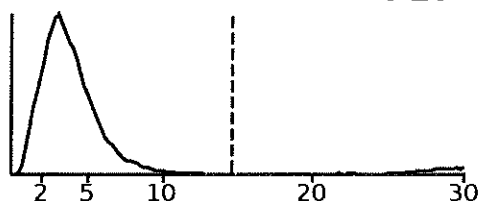

RESULTS

ANIMAL NAME: B12lr eob

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:16

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:922757

PLATE ID:01980922757

OPERATOR ID:

LAB.:

TEST TIME:2023-04-06 14:37

MACHINE ID:120007423

PRINT TIME:2023-04-06 14:37

Ver:V1.00.00.87/1.00.01.44



Assay	Result	Ref	Low	Normal	High
ALB	2.2g/dL	L 2.2–3.7			
TP	3.8g/dL	L 5.5–7.2			
GLOB	1.6g/dL	1.5–2.8			
A/G	1.31				
TB	<0.1mg/dL	L 0.3–0.8			
GGT	11U/L	0–14			
AST	318U/L	H 0–98			
ALT	92U/L	H 31–53			
ALP	94U/L	70–145			
TBA	3.48umol/L				
AMY	187U/L	L 200–378			
LPS	38U/L				
LDH	704U/L	H 34–129			
CK	> 4000U/L	H 218–2705			
Crea	0.7mg/dL	L 0.8–1.8			
UA	<10umol/L	0–130			
BUN	22.15mg/dL	10.12–24.17			
BUN/CREA	129.398	21.000–236.000			
GLU	227.21mg/dL	H 75.14–145.24			
TC	74.72mg/dL	H 34.65–52.75			
TG	188.49mg/dL	H 26.10–153.12			
tCO2	17.4mmol/L	13.0–22.0			
Ca	10.12mg/dL	5.60–12.00			
PHOS	4.33mg/dL	1.21–4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

0262G6272

RESULTS

ANIMAL NAME:Blr12_eob

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:15

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:9220185

PLATE ID:006509220185

OPERATOR ID:

LAB.:

TEST TIME:2023-04-06 14:25

MACHINE ID:120007423

PRINT TIME:2023-04-06 14:25

Ver:V1.00.00.87/1.00.01.44




Assay	Result	Ref	Low	Normal	High
APTT	96.8s				
PT	19.2s				
TT	23.1s				
Fib	1.63g/L				

WAT:1

EMP:0

CHE:0

2577H5538

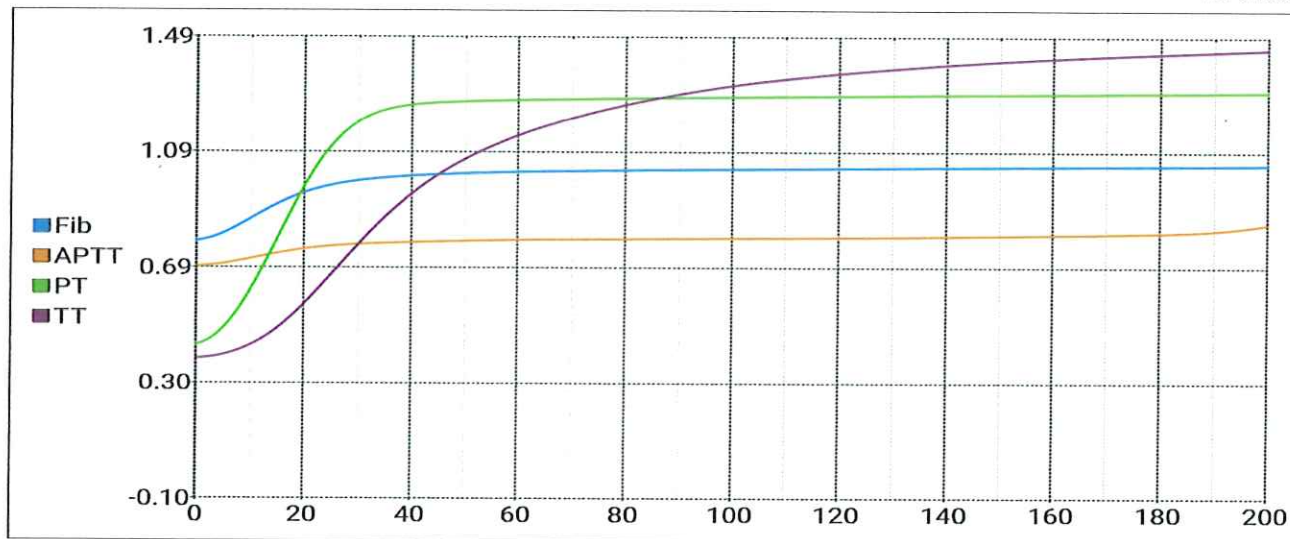

Note: The project curves from top to bottom are:Fib,APTT,PT,TT.

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004 10:38 AM 4/7/2023
 PATIENT REPORT Syringe - S 65uL Sample # 16418

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type Not specified
 T 37.0 °C

Blood gas values

pH	7.388		[	-	]
pCO ₂	47.0	mmHg	[	-	]
pO ₂	26.5	mmHg	[	-	]

Oximetry values

ctHb	7.4	g/dL	[	-	]
Hct _c	22.7	%			
sO ₂	32.4	%	[	-	]
FO ₂ Hb	31.2	%	[	-	]
FCOHb	2.8	%	[	-	]
FHHb	65.2	%	[	-	]
FMethHb	0.8	%	[	-	]

Electrolyte values

cK ⁺	4.7	meq/L	[	-	]
cNa ⁺	142	meq/L	[	-	]
cCa ²⁺	3.09	meq/L	[	-	]
cCl ⁻	99	meq/L	[	-	]

Metabolite values

cGlu	155	mg/dL	[	-	]
cLac	9.1	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	28.3	mmol/L
p50 _c	35.37	mmHg
ABE _c	2.9	mmol/L

Notes

c Calculated value(s)

Solution pack lot: NE-33 Sensor cassette run #: 2575-8
 Printed 10:38:08AM 4/7/2023

RESULT

Animal ID B12LR	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		
Sample ID 24HR	Analysis Date 04/07/2023 10:21:52	Operator JOY

Analyser Alarms			Analysis Alarms		XB

RESULTS



ANIMAL NAME: B12LR 24hrs

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 14

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220126

PLATE ID: 019809220126

OPERATOR ID:

LAB.:

TEST TIME: 2023-04-07 11:49

MACHINE ID: 120007423

PRINT TIME: 2023-04-07 11:50

Ver: V1.00.00.87/1.00.01.44

Assay	Result	Ref	Low	Normal	High
ALB	2.4g/dL	2.2-3.7			
TP	4.5g/dL	L 5.5-7.2			
GLOB	2.1g/dL	1.5-2.8			
A/G	1.14				
TB	0.1mg/dL	L 0.3-0.8			
GGT	8U/L	0-14			
AST	569U/L	H 0-98			
ALT	305U/L	H 31-53			
ALP	125U/L	70-145			
TBA	4.29umol/L				
AMY	289U/L	200-378			
LPS	34U/L				
LDH	913U/L	H 34-129			
CK	> 4000U/L	H 218-2705			
Crea	0.4mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	16.63mg/dL	10.12-24.17			
BUN/CREA	150.932	21.000-236.000			
GLU	150.53mg/dL	H 75.14-145.24			
TC	130.14mg/dL	H 34.65-52.75			
TG	528.56mg/dL	H 26.10-153.12			
tCO2	20.2mmol/L	13.0-22.0			
Ca	12.32mg/dL	H 5.60-12.00			
PHOS	4.70mg/dL	1.21-4.90			

CK> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

1162E2601

RADIOMETER ABL90 SERIES

ABL90 I393-090R0199N0004
 PATIENT REPORT Syringe - S 65uL 10:11 AM 4/8/2023
 Sample # 16459

Identifications

Patient ID
 Patient last name
 Patient first name
 Sample type T Not specified
 37.0 °C

Blood gas values

pH	7.306		[	-	]
pCO ₂	48.7	mmHg	[	-	]
pO ₂	27.5	mmHg	[	-	]

Oximetry values

ctHb	6.0	g/dL	[	-	]
Hct _c	18.3	%			
sO ₂	29.7	%	[	-	]
FO ₂ Hb	28.7	%	[	-	]
FCOHb	2.9	%	[	-	]
FHHb	67.8	%	[	-	]
FMethHb	0.6	%	[	-	]

Electrolyte values

cK ⁺	5.0	meq/L	[	-	]
cNa ⁺	144	meq/L	[	-	]
cCa ²⁺	3.36	meq/L	[	-	]
cCl ⁻	105	meq/L	[	-	]

Metabolite values

cGlu	146	mg/dL	[	-	]
cLac	8.7	mmol/L	[	-	]

Calculated values

cHCO ₃ ⁻ (P) _c	24.3	mmol/L
p50 _c	38.50	mmHg
ABE _c	-1.9	mmol/L

Notes

c Calculated value(s)

Solution pack lot: NE-33
 Printed 10:11:44AM 4/8/2023
 Sensor cassette run #: 2575-485

RESULT

Animal ID B12LR	Owner name	Owner first name
Name	Species Rabbit	
Date of birth		
Sample ID 48HRS	Analysis Date 04/08/2023 09:54:35	Operator MEB

Analyser Alarms Analysis Alarms

SCH, XB, CPLT

WBC 1.4 L $10^3/\text{mm}^3$ **Normal range** 2.5 13.8

LYM% --- %

MON% --- %

GRA% --- %

(EOS%) --- %


LYM# --- $10^3/\text{mm}^3$

MON# --- $10^3/\text{mm}^3$

GRA# --- $10^3/\text{mm}^3$

EOS# --- $10^3/\text{mm}^3$

WBC

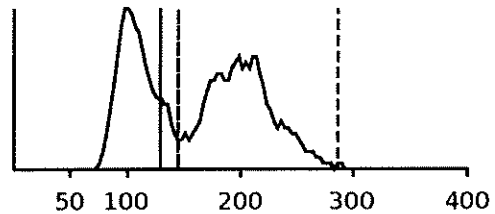

RBC 0.54 L $10^6/\text{mm}^3$ 4.80 7.20

HGB 1.2 L g/dl 10.6 16.0

HCT 3.4 L % 33.9 50.1


MCV 62 μm^3 62 79

MCH 22.8 pg 19.0 25.6

MCHC 36.6 H g/dl 28.4 35.0

RDW --- %


RBC

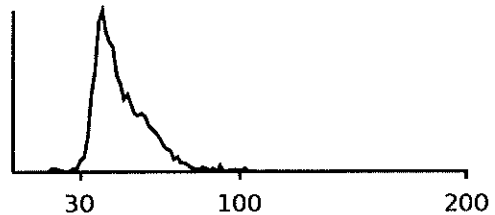

PLT 97 $10^3/\text{mm}^3$ 0 962

MPV --- μm^3

PLT

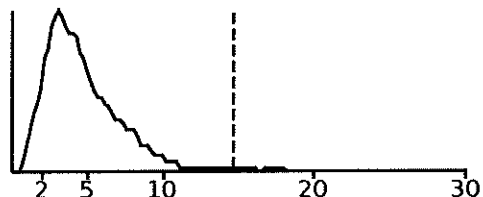

RESULTS

ANIMAL NAME:48h B12LR

OWNER NAME:

Animal:Rabbit

Medical ID:

SAMPLE ID:3

AGEGroup:Juvenile

SAMPLE TYPE:Whole Blood

REAGENT BATCH NO.:9220203

PLATE ID:019809220203

OPERATOR ID:

LAB.:

TEST TIME:2023-04-08 11:13

MACHINE ID:120007423

PRINT TIME:2023-04-08 11:14

Ver:V1.00.00.87/1.00.01.44



Assay	Result	Ref	Low	Normal	High
ALB	2.2g/dL	L 2.2-3.7			
TP	4.6g/dL	L 5.5-7.2			
GLOB	2.5g/dL	1.5-2.8			
A/G	0.88				
TB	<0.1mg/dL	L 0.3-0.8			
GGT	9U/L	0-14			
AST	365U/L	H 0-98			
ALT	334U/L	H 31-53			
ALP	104U/L	70-145			
TBA	2.62umol/L				
AMY	416U/L	H 200-378			
LPS	47U/L				
LDH	600U/L	H 34-129			
CK	2202U/L	218-2705			
Crea	0.6mg/dL	L 0.8-1.8			
UA	<10umol/L	0-130			
BUN	17.78mg/dL	10.12-24.17			
BUN/CREA	128.347	21.000-236.000			
GLU	142.70mg/dL	75.14-145.24			
TC	142.02mg/dL	H 34.65-52.75			
TG	> 609.00mg/dL	H 26.10-153.12			
tCO2	18.5mmol/L	13.0-22.0			
Ca	11.95mg/dL	5.60-12.00			
PHOS	4.82mg/dL	1.21-4.90			

TG> detection limit. Please dilute sample and re-test

WAT:0

EMP:0

CHE:0

5183H6841

RESULTS

ANIMAL NAME: B12lr 48hr

OWNER NAME:

Animal: Rabbit

Medical ID:

SAMPLE ID: 4

AGE Group: Juvenile

SAMPLE TYPE: Whole Blood

REAGENT BATCH NO.: 9220185

PLATE ID: 006509220185

OPERATOR ID:

LAB.:

TEST TIME: 2023-04-08 11:30

MACHINE ID: 120007423

PRINT TIME: 2023-04-08 11:30

Ver: V1.00.00.87/1.00.01.44




Assay	Result	Ref	Low	Normal	High
APTT	107.6s				
PT	7.3s				
TT	18.3s				
Fib	3.40g/L				

WAT:0

EMP:0

CHE:0

1737D7817

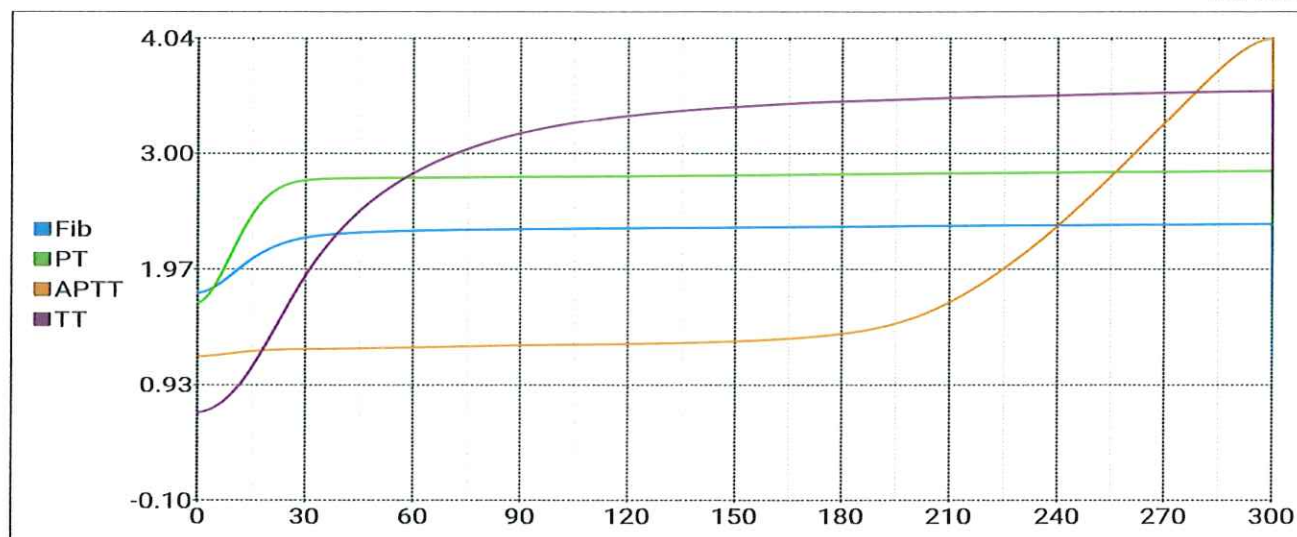

Note: The project curves from top to bottom are: Fib, PT, APTT, TT.