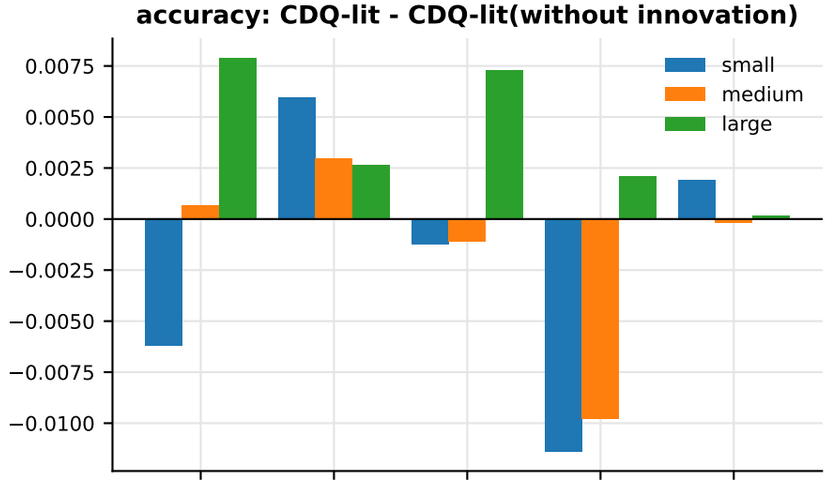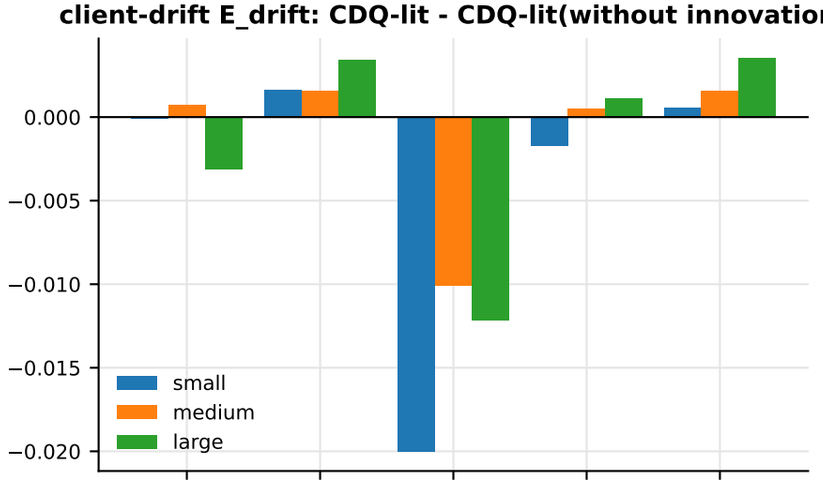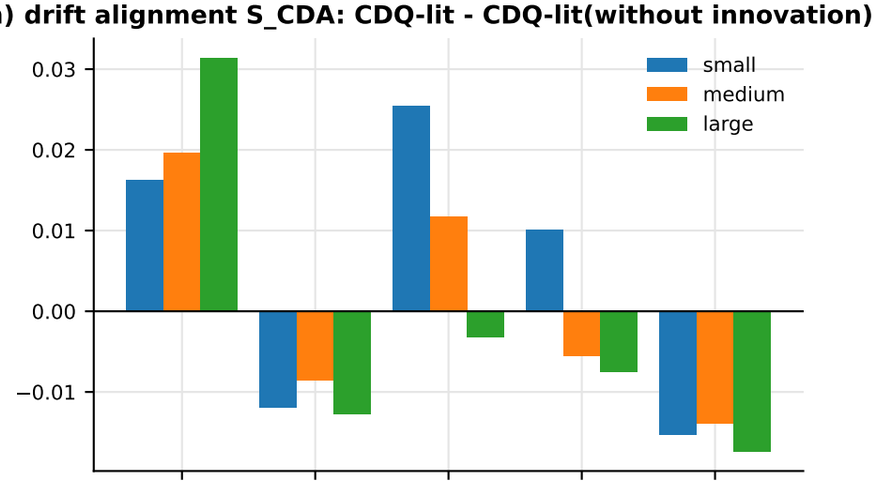Ablation (I1 DMapS-FSNR+pinning, I2 R-FD, I3a DR-JPS, I3b Fed-QDrift, I4 FD-SIC). accuracy/S_CDA: >0 means the innovation helps; E_drift: <0 means it helps