
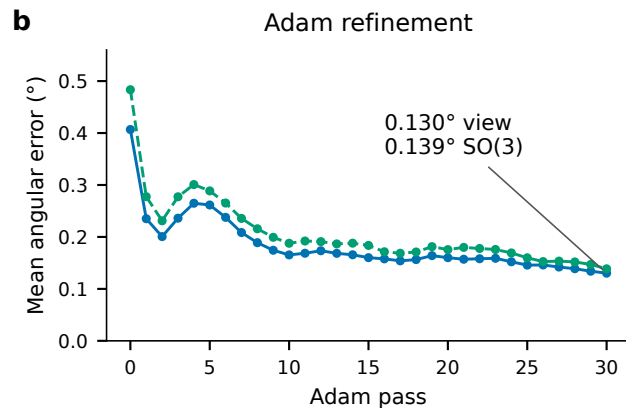




80S | fixed external density | 64 particles

—●— Viewing direction - - - ● - - - Full SO(3)

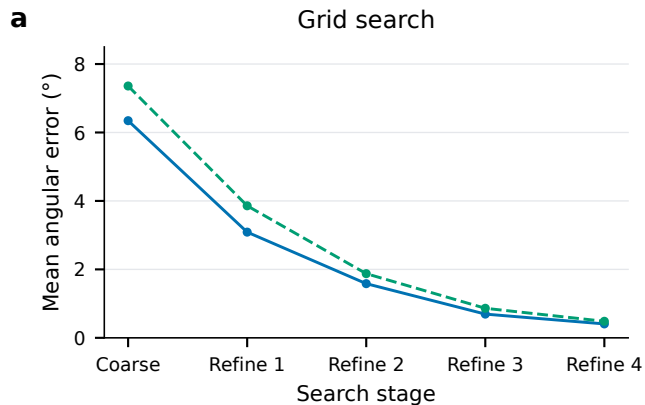

1AKE | pose recovery remains inaccurate | 103 evaluation particles

— CryoDyna-optpose - - - Random SO(3) — DRGN-AI

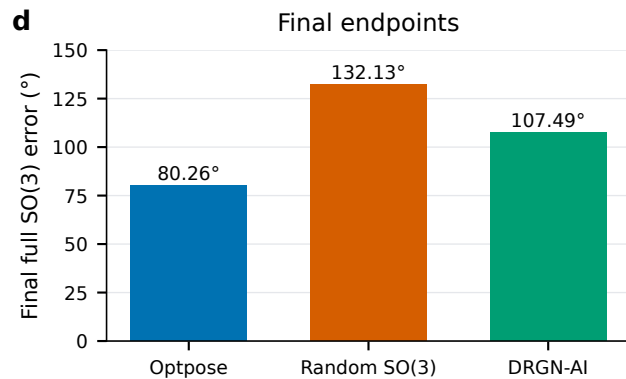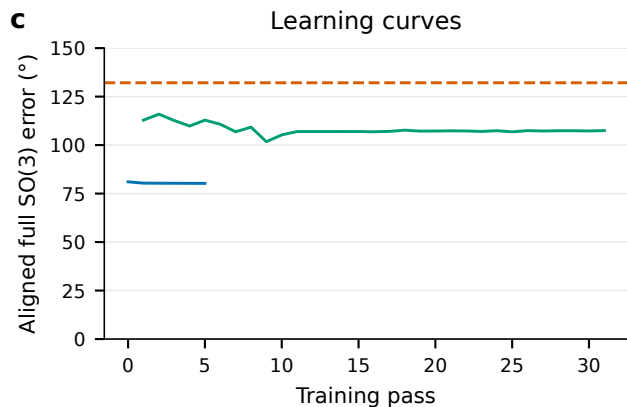

80S: per-stage global alignment; panel a/b use different error ranges.

1AKE: 25 gauge-fit particles; actual method budgets retained. 80S DRGN-AI evaluation pending.