

Standard Name 90 of 90

↑

20A 0494-1 ID

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal  
Date: 16-Jul-20 Time: 16:00:37

Batch Name 1 of 1

↑

FA21-ITN-B101 DKI18362 1-1 3012673/II/21 VIC

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal  
Date: 27-May-21 Time: 15:41:40


CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: ( 2.00 1.00)

Delta 

D65 / 10

F11 / 10

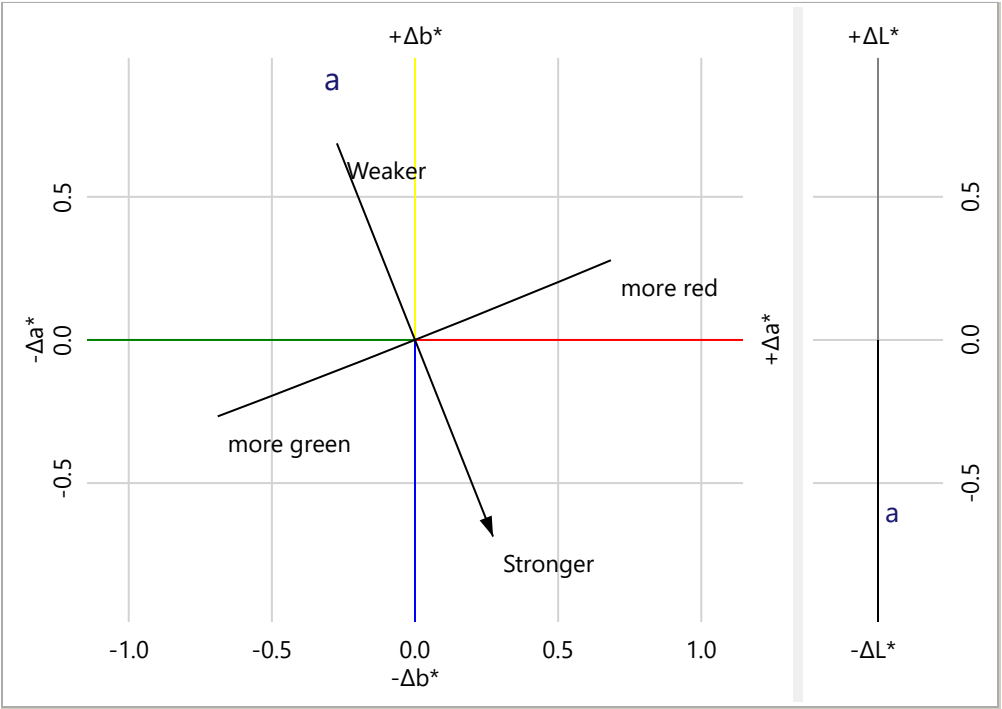

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
FA21-ITN-B101 DKI18362 1-1 3012673/II/21 VIOLET	D65 10 Deg	-0.58	-0.30	0.94	-0.30	-0.41	0.05	0.51		Pass	darker	less saturated more red
FA21-ITN-B101 DKI18362 1-1 3012673/II/21 VIOLET	F11 10 Deg	-0.57	-0.13	1.09	-0.31	-0.43	0.10	0.54	0.14	Pass	darker	less saturated more red