

Standard Name 66 of 66

↑

21A 0370-1 AD

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 22-Jun-21 Time: 15:07:43

Batch Name 1 of 1

↑

FA22-ITN-S106 DKI18362 1-1 3037127/V/21.

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 22-Jun-21 Time: 15:09:15

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

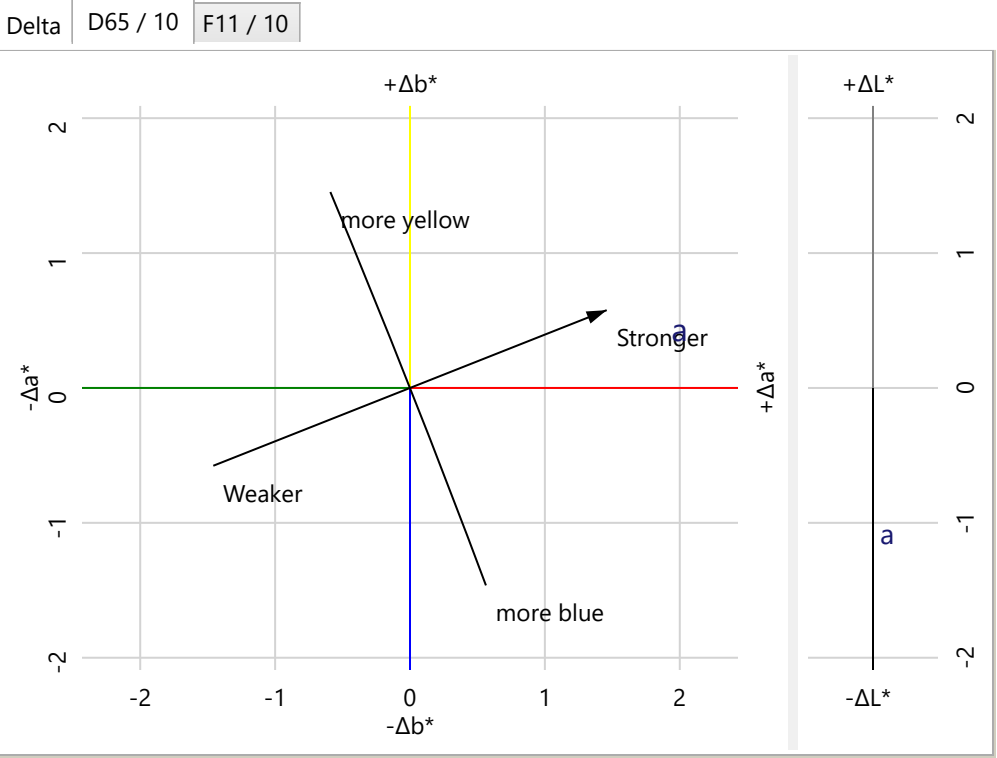

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

<u>Batch Name</u>	<u>III/Obs</u>	<u>DL*</u>	<u>Da*</u>	<u>Db*</u>	<u>DL*/ISL</u>	<u>DC*/cSC</u>	<u>DH*/SH</u>	<u>CMC DE</u>	<u>M.I.</u>	<u>P/E</u>	<u>Color</u>	<u>Comments</u>	
FA22-ITN-S106 DKI18362 1-1 3037127/V/21.	D65 10 Deg	-1.05	1.99	0.49	-0.43	0.64	-0.15	0.78		Warn	too dark	too bright	too blue
FA22-ITN-S106 DKI18362 1-1 3037127/V/21.	F11 10 Deg	-0.85	1.16	0.58	-0.33	0.40	-0.01	0.52	1.12	Pass	too dark	too bright	too blue