

Standard Name 86 of 105

DataColor TOOLS 2.4.4

S/N NO. 8823242

20C 0655 CRD

Visual Hue Request:

New Std Retrieve Std Store Std List Std Update Std

Instrument Setup: %R LAV SCI UV Cal

Date: 24-Jun-20 Time: 08:48:46

Batch Name 3 of 3

BKJ FA21 SJS7091 1-1 3015244/III/21

New Bat Retrieve Bat Store Bat List Bat Update Bat


Instrument Setup: %R LAV SCI UV Cal

Date: 26-Apr-21 Time: 14:48:08

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: ( 2.00 1.00)

Delta D65 / 10 F11 / 10 A / 10

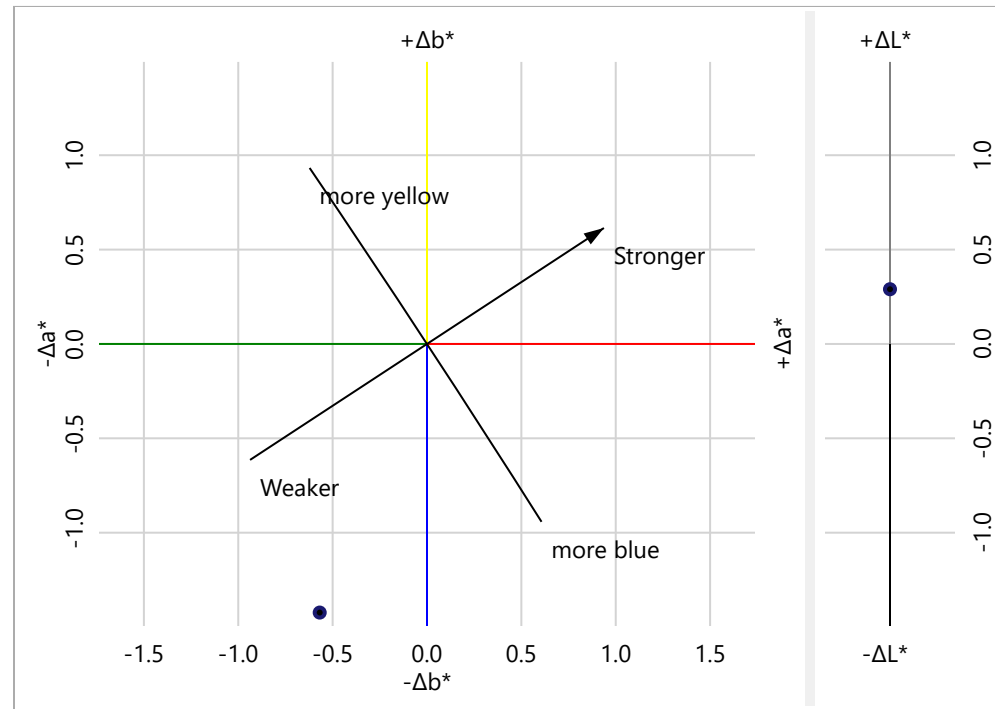

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form

Batch Name

III/Obs

DL\*

Da\*

Db\*

DL\*/ISL

DC\*/cSC

DH\*/SH

CMC DE

M.I.

P/E

Color Comments

BKJ FA21 SJS7091 1-1 3015244/III/21	D65 10 Deg	0.29	-0.58	-1.42	0.13	-0.42	-0.58	0.73		Pass	lighter	less saturated	more blue
BKJ FA21 SJS7091 1-1 3015244/III/21	F11 10 Deg	0.17	-0.84	-1.68	0.08	-0.56	-0.56	0.80	0.36	Warn	lighter	less saturated	more blue
BKJ FA21 SJS7091 1-1 3015244/III/21	A 10 Deg	0.19	-0.33	-1.59	0.08	-0.43	-0.67	0.80	0.45	Warn	lighter	less saturated	more red