

Standard Name

8 of 28

↑

AE6M Focus OliveF21

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Instrument Setup: %R LAV SCI UV Cal

Date: 12-Apr-21Time: 10:39:43

Batch Name

4 of 4

↑

70011247 CM31-2021-284326 1-1 3021993

↓

New Bat

Retrieve Bat


Store Bat

List Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 25-Apr-21Time: 09:55:58

Batch Name
70011247 CM31-2021-284326 1-1 3021993/IV/21
70011247 CM31-2021-284326 1-1 3021993/IV/21

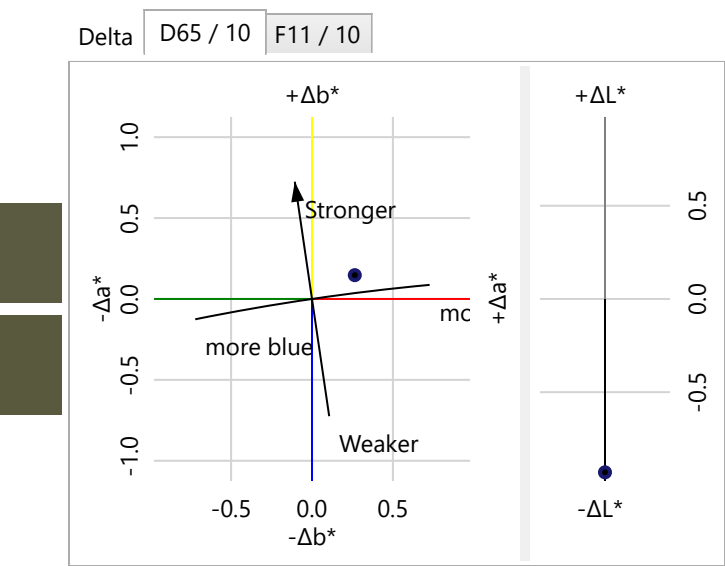

Single/All

Zoom In

Zoom Out

CMC Plot

Print Form

Standard %R						
400-450nm	11.16	9.05	7.72	6.59	6.02	5.93
460-510nm	6.03	6.51	7.75	9.04	9.86	10.33
520-570nm	11.02	11.70	11.73	11.50	11.01	10.62
580-630nm	10.43	10.36	10.39	10.44	10.78	11.61
640-690nm	13.37	16.10	19.70	24.02	29.09	33.60
700nm	39.67					

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: ( 2.00 1.00)

Ill/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
D65 10 Deg	-0.93	0.26	0.15	-0.49	0.08	-0.32	0.59		Pass	darker	more saturated more yellow
F11 10 Deg	-0.80	0.58	0.22	-0.42	0.06	-0.63	0.76	0.34	Warn	darker	more saturated more yellow