

Standard Name 6 of 6

↑

21C 0400-1.ARL

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 28-Nov-21 Time: 14:06:37

Batch Name 2 of 3

↑

R1117235 5484629 1-1 3078087/X/21 RESUBM

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 15-Dec-21 Time: 11:13:48

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)


Measured by:

Delta

D65 / 10

F11 / 10

A / 10

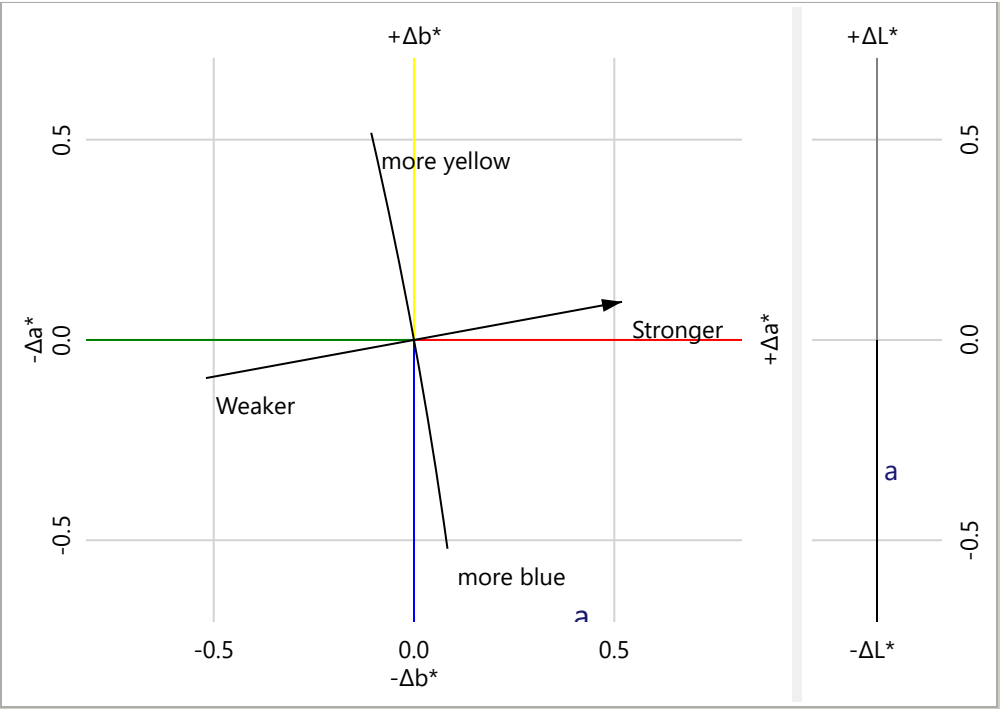

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
R1117235 5484629 1-1 3078087/X/21 RESUBMIT	D65 10 Deg	-0.31	0.41	-0.67	-0.11	0.24	-0.85	0.89		Warn	too dark	too bright	too blue
R1117235 5484629 1-1 3078087/X/21 RESUBMIT	F11 10 Deg	-0.32	0.47	-0.72	-0.11	0.22	-0.95	0.98	0.08	Warn	too dark	too bright	too blue
R1117235 5484629 1-1 3078087/X/21 RESUBMIT	A 10 Deg	-0.30	0.38	-0.65	-0.11	0.11	-0.90	0.91	0.04	Pass	too dark	too bright	too blue