

Standard Name 13 of 13

↑

9C 0293 CRD

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 23-May-19 Time: 13:48:16

Batch Name 1 of 3

↑

F3T18157 5484629 6-1 3078087/X/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV 400


Date: 28-Nov-21 Time: 13:44:51

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
F3T18157 5484629 6-1 3078087/X/21	D65 10 Deg	1.06	0.15	-0.04	0.76	0.05	0.22	0.79		Warn	too light	too bright	too red
F3T18157 5484629 6-1 3078087/X/21	F11 10 Deg	1.02	-0.44	-0.16	0.74	0.51	-0.37	0.97	0.57	Warn	too light	too bright	too green
F3T18157 5484629 6-1 3078087/X/21	A 10 Deg	1.09	0.57	0.02	0.79	0.57	0.53	1.11	0.38	Pass	too light	too bright	too red

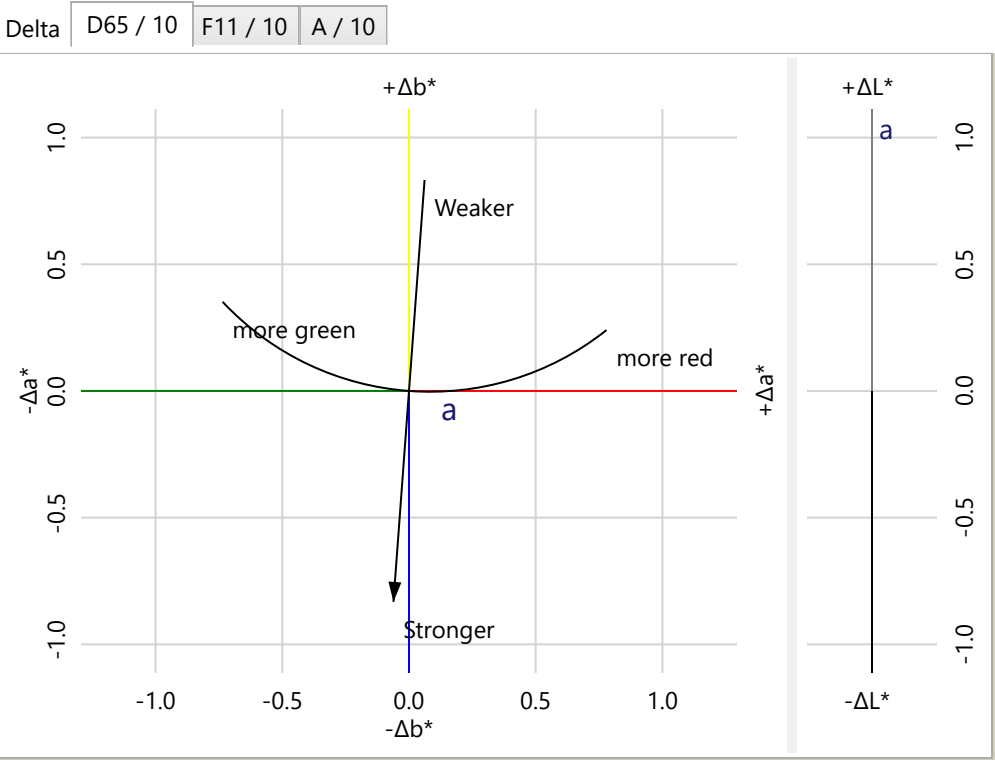

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form