

Standard Name145 of 177

↑

5A 1151 AD/FBM15042(MSH)/STD MIZUNO 8-8

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 13-Aug-18Time: 19:40:56

Batch Name1 of 1

↑

FA21-ITN-B109 R1113457 1-1 3016517/III/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat


Instrument Setup: %R LAV SCI UV Cal

Date: 05-Apr-21Time: 10:53:27

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

DeltaD65 / 10F11 / 10

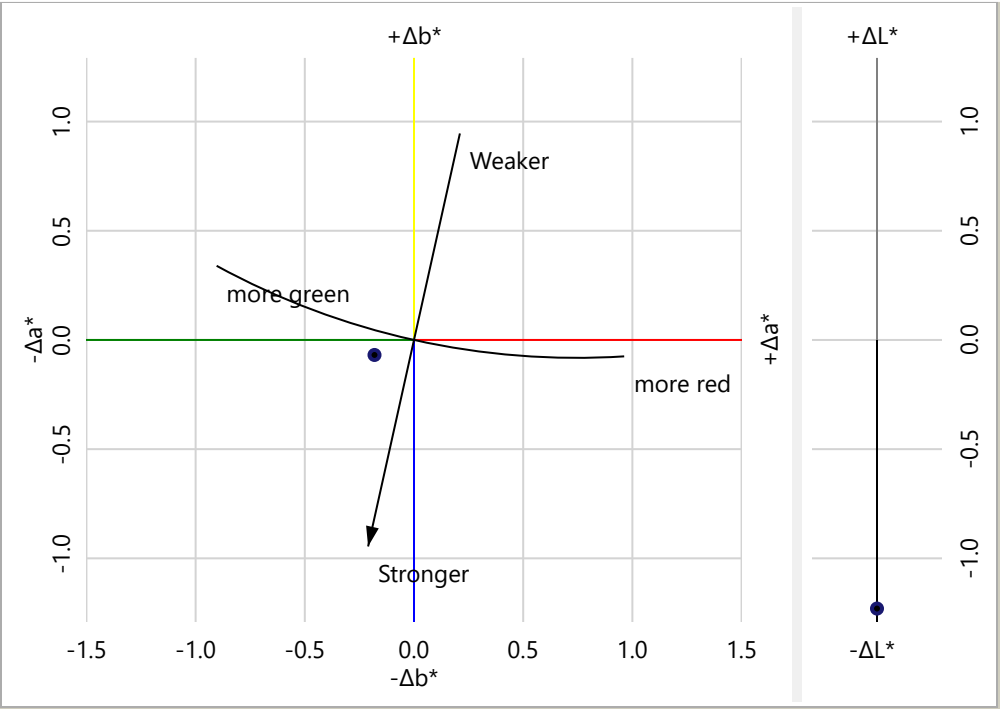

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
FA21-ITN-B109 R1113457 1-1 3016517/III/21	D65 10 Deg	-1.23	-0.18	-0.07	-0.68	0.13	-0.21	0.73		Warn	darker	more saturated more green
FA21-ITN-B109 R1113457 1-1 3016517/III/21	F11 10 Deg	-1.30	0.05	-0.15	-0.73	0.17	0.08	0.75	0.28	Warn	darker	more saturated more red