

Standard Name 83 of 239

↑

18157/220331L-B

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV SCI UV Cal

Date: 13-Jun-22 Time: 13:51:45

Batch Name 2 of 3

↑

B22203801AA-001 1-1 3058451/X/22LILAC SMO

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal


Date: 27-Oct-22 Time: 10:04:52

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments			
R1117235 B22203801AA-001 1-1 3058451/X/22LILAC SMO	D65 10 Deg	-1.09	-0.17	0.63	-0.43	-0.38	0.03	0.57		Pass	too dark	too dull	too red	
R1117235 B22203801AA-001 1-1 3058451/X/22LILAC SMO	F11 10 Deg	-1.07	-0.27	0.60	-0.43	-0.35	-0.12	0.56	0.14	Pass	too dark	too dull	too green	
R1117235 B22203801AA-001 1-1 3058451/X/22LILAC SMO	A 10 Deg	-1.05	-0.37	0.74	-0.42	-0.44	-0.31	0.68	0.29	Pass	too dark	too dull	too green	

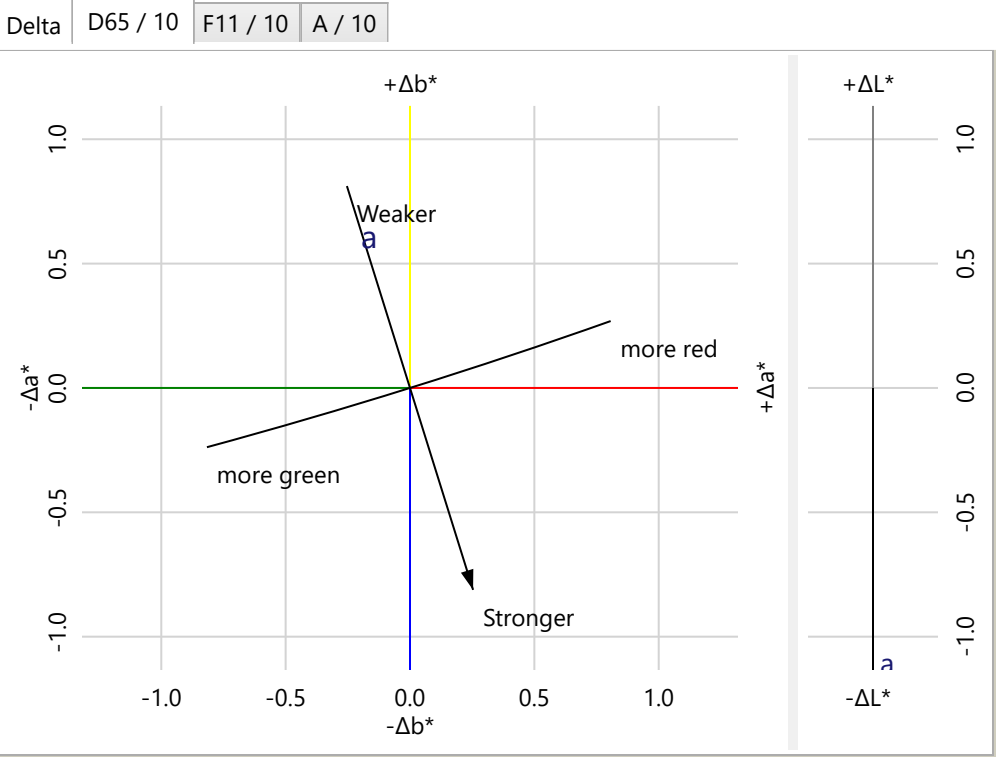

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form