

Standard Name146 of 175

↑

5A 1152 ASC/FBM15042(MSH)/DARK NAVY(14I

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 03-Dec-20Time: 09:21:50

Batch Name1 of 1

↑

FA21-ITN-B109 R1113457 1-1 3016517/III/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat


Instrument Setup: %R LAV SCI UV Cal

Date: 05-Apr-21Time: 10:45:45

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

DeltaD65 / 10F11 / 10

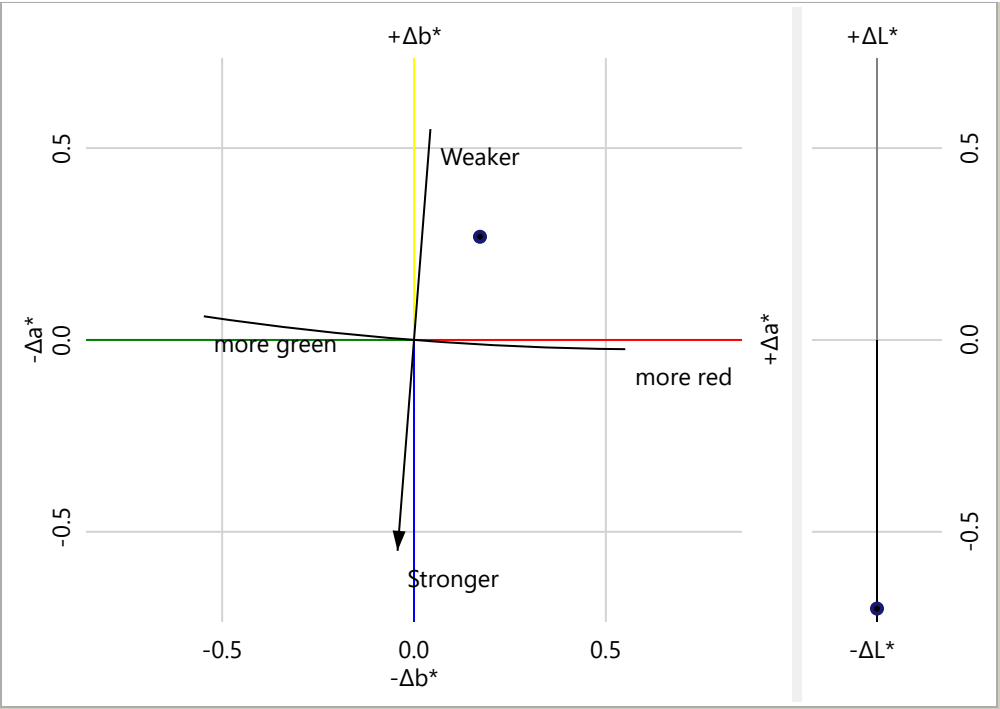

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
FA21-ITN-B109 R1113457 1-1 3016517/III/21	D65 10 Deg	-0.70	0.17	0.26	-0.62	-0.25	0.20	0.70		Warn	darker	less saturated more red
FA21-ITN-B109 R1113457 1-1 3016517/III/21	F11 10 Deg	-0.60	0.32	0.36	-0.56	-0.33	0.36	0.74	0.18	Warn	darker	less saturated more red