

Standard Name176 of 176

↑

5A 1152 ASC /FBM15042(FLT)/DARK NAVY(140

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 09-Aug-18Time: 20:40:50

Batch Name1 of 1

↑

FA21-ITN-B108 FBM15293 3-1 3015961/II/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 05-Apr-21Time: 10:50:39

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

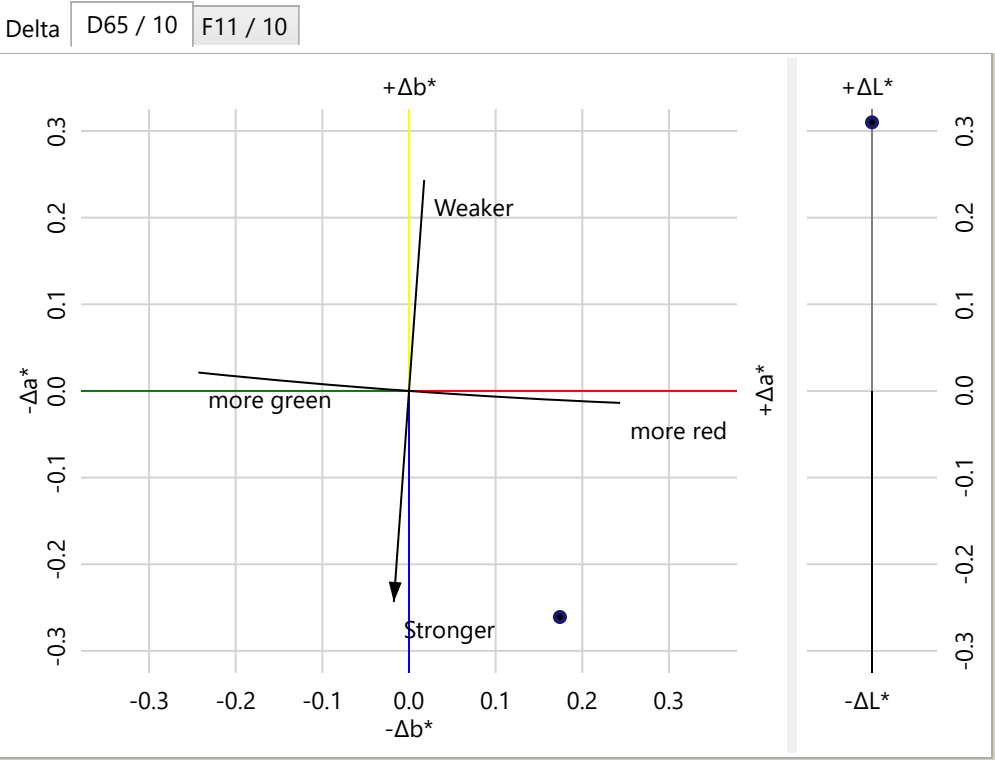

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

| Batch Name | III/Obs | DL* | Da* | Db* | DL*/ISL | DC*/cSC | DH*/SH | CMC DE | M.I. | P/E | Color | Comments |
|--|------------|------|------|-------|---------|---------|--------|--------|------|------|---------|-------------------------|
| FA21-ITN-B108 FBM15293 3-1 3015961/II/21 | D65 10 Deg | 0.32 | 0.17 | -0.26 | 0.29 | 0.23 | 0.25 | 0.45 | | Pass | lighter | more saturated more red |
| FA21-ITN-B108 FBM15293 3-1 3015961/II/21 | F11 10 Deg | 0.39 | 0.31 | -0.30 | 0.37 | 0.23 | 0.44 | 0.62 | 0.17 | Warn | lighter | more saturated more red |