

Standard Name 48 of 48

↑

Capture Blue CAPB

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 09-Sep-20 Time: 10:50:33

Batch Name 1 of 1

↑

PR2021/622509 F3T18157 2-1 3012062/II/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 17-Apr-21 Time: 10:23:27

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

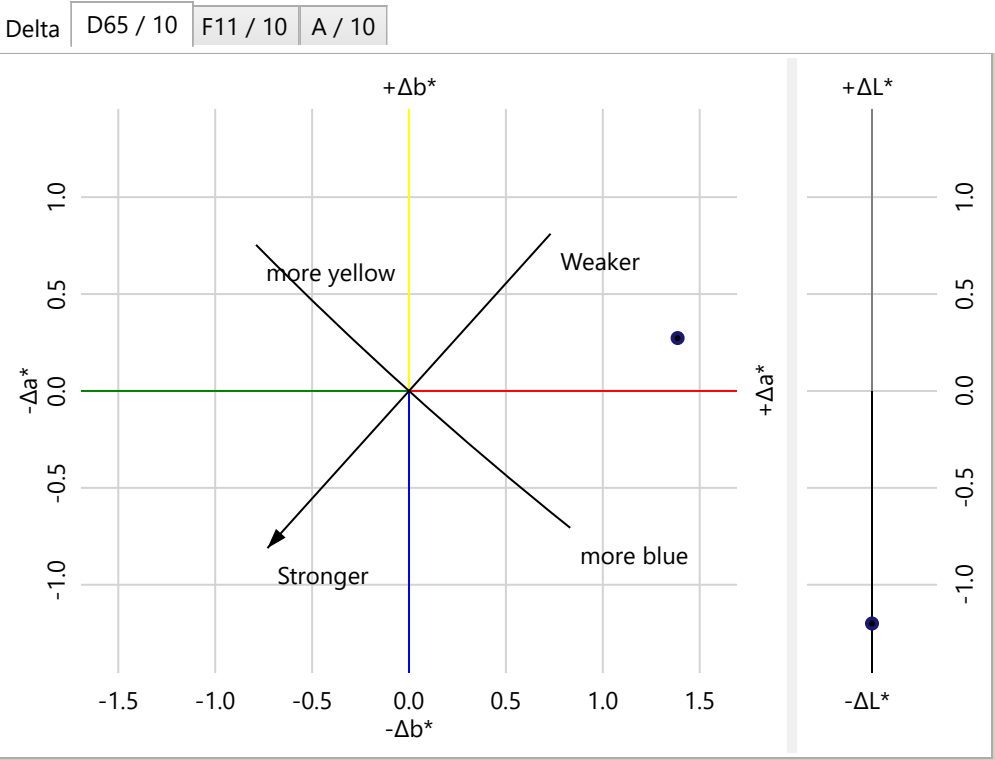

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
PR2021/622509 F3T18157 2-1 3012062/II/21	D65 10 Deg	-1.20	1.38	0.27	-0.62	-0.69	0.76	1.20		Fail	darker	less saturated more blue
PR2021/622509 F3T18157 2-1 3012062/II/21	F11 10 Deg	-1.11	0.62	0.36	-0.59	-0.38	0.30	0.77	0.70	Warn	darker	less saturated more red
PR2021/622509 F3T18157 2-1 3012062/II/21	A 10 Deg	-1.01	1.15	0.89	-0.54	-0.78	0.33	1.01	0.58	Fail	darker	less saturated more blue