

↑

20B 0177-2 DRSC

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal
Date: 26-Aug-21 Time: 17:05:41

↑

MTR17080 BOOKING FA22 4-2 3088202/XII/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat


Instrument Setup: %R LAV SCI UV Cal
Date: 09-Jan-22 Time: 09:28:31

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
MTR17080 BOOKING FA22 4-2 3088202/XII/21	D65 10 Deg	0.10	-0.49	0.25	0.10	-0.15	-0.70	0.72		Pass	too light	too dull	too green
MTR17080 BOOKING FA22 4-2 3088202/XII/21	F11 10 Deg	0.04	-0.40	0.16	0.04	-0.07	-0.56	0.56	0.13	Pass	too light	too dull	too green
MTR17080 BOOKING FA22 4-2 3088202/XII/21	A 10 Deg	0.07	-0.29	0.15	0.07	-0.13	-0.41	0.43	0.22	Pass	too light	too dull	too green

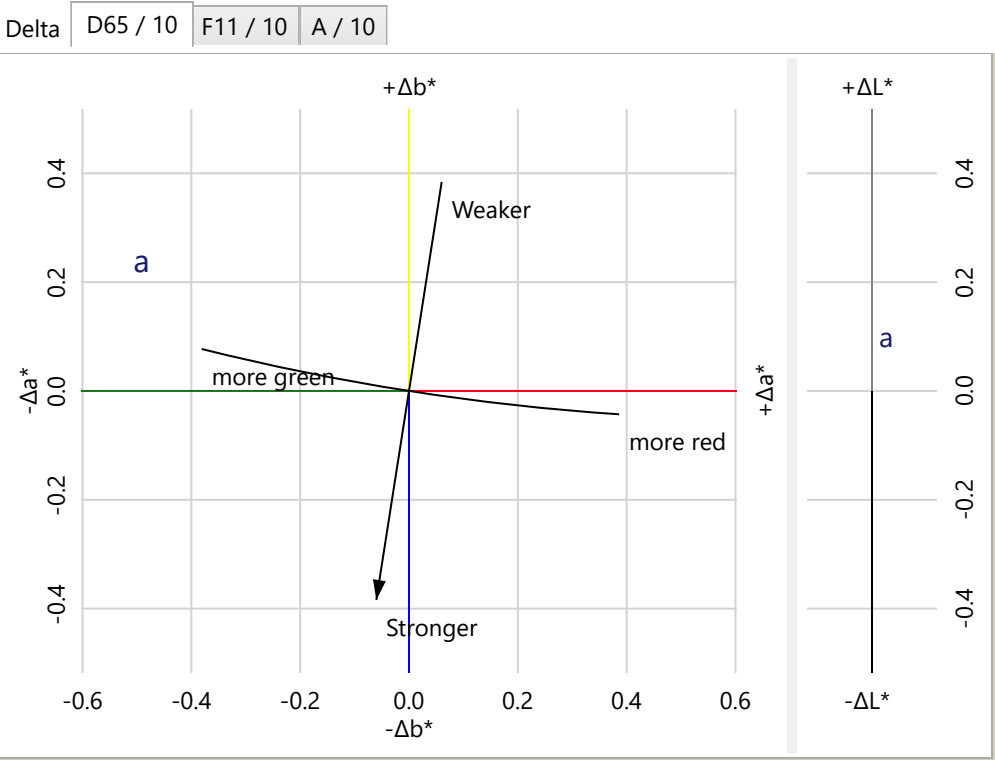

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form