

Standard Name 113 of 164

↑

20C 1222 BRD

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 21-Feb-21 Time: 08:58:47

Batch Name 1 of 1

↑

2210001AA-003 34218 DOM2201871 CRIMSON

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat


Instrument Setup: %R LAV SCI UV Cal

Date: 08-Nov-22 Time: 15:00:50

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: ( 2.00 1.00)

Measured by:

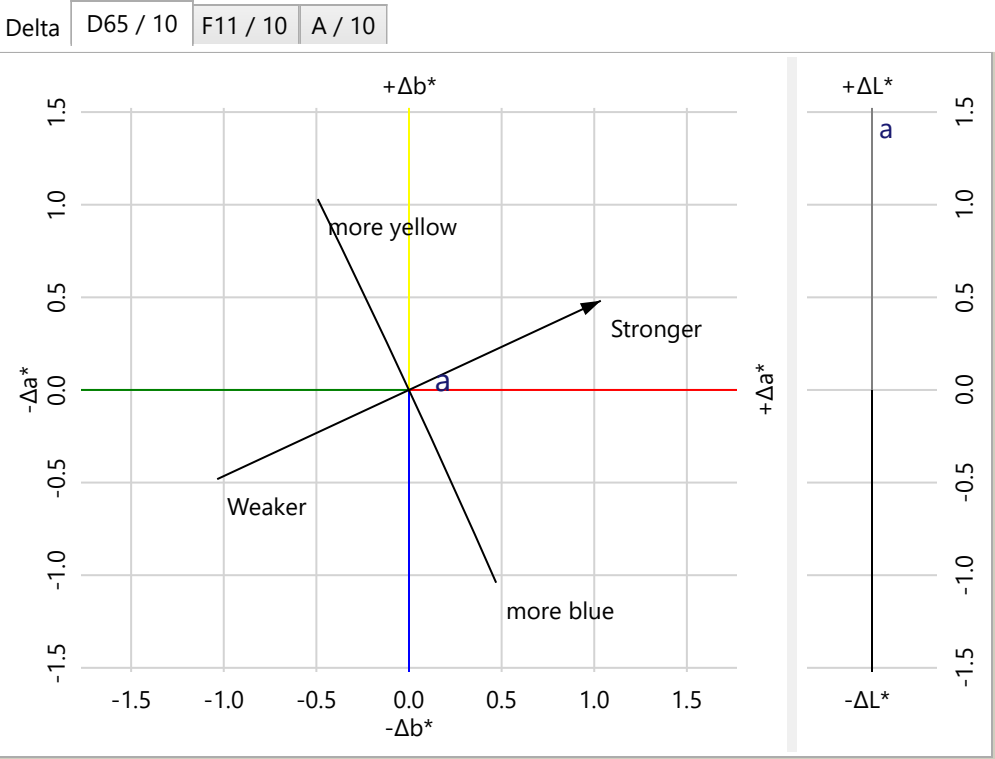

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/F	Color	Comments	
SJS7091 B22210001AA-003 34218 DOM2201871 CRIMSON	D65 10 Deg	1.45	0.18	0.10	0.80	0.08	0.01	0.81		Warn	too light	too bright	too yellow
SJS7091 B22210001AA-003 34218 DOM2201871 CRIMSON	F11 10 Deg	1.42	0.33	0.11	0.74	0.13	-0.06	0.75	0.33	Warn	too light	too bright	too blue
SJS7091 B22210001AA-003 34218 DOM2201871 CRIMSON	A 10 Deg	1.47	0.25	0.08	0.73	0.09	-0.07	0.74	0.47	Pass	too light	too bright	too blue