

Standard Name 6 of 6

↑

21C 0400-1.ARL

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV SCI UV 400

Date: 28-Nov-21 Time: 14:06:37

Batch Name 3 of 3

↑

SJS7091 5484629 1-1 3078087/X/21 RESUBMIT

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal

Date: 15-Dec-21 Time: 11:17:51

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: ( 2.00 1.00)


Measured by:

Delta 

D65 / 10

F11 / 10

A / 10

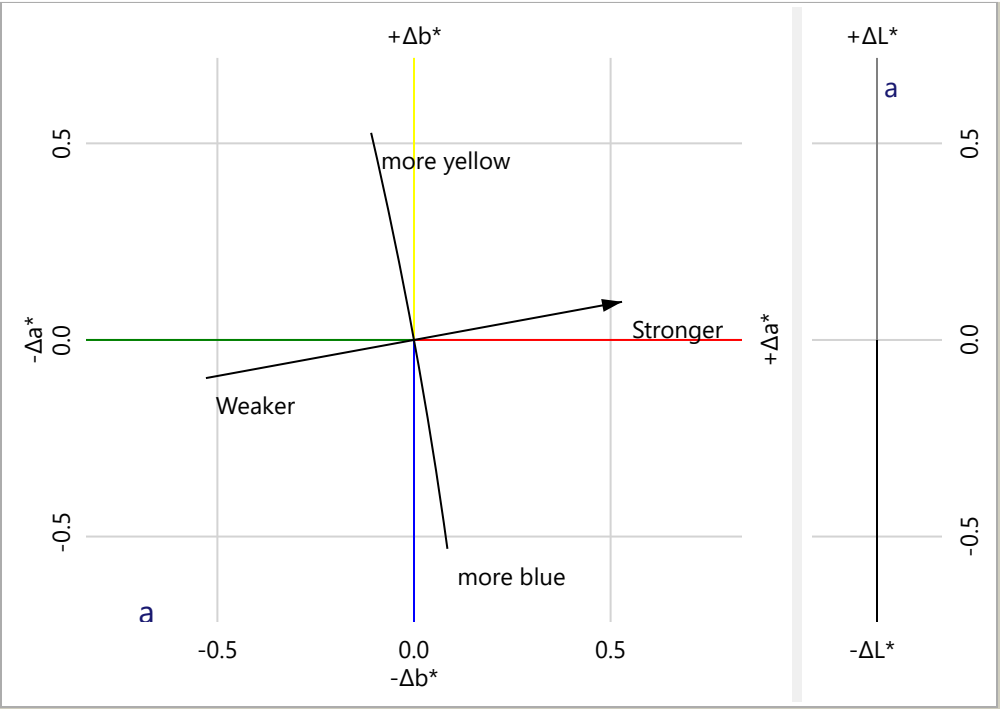

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
SJS7091 5484629 1-1 3078087/X/21 RESUBMIT	D65 10 Deg	0.67	-0.69	-0.67	0.24	-0.61	-0.65	0.92		Warn	too light	too dull	too blue
SJS7091 5484629 1-1 3078087/X/21 RESUBMIT	F11 10 Deg	0.56	-0.78	-0.87	0.20	-0.71	-0.78	1.07	0.25	Warn	too light	too dull	too blue
SJS7091 5484629 1-1 3078087/X/21 RESUBMIT	A 10 Deg	0.54	-0.89	-0.88	0.19	-0.82	-0.65	1.06	0.33	Pass	too light	too dull	too blue