

Standard Name53 of 53

↑

Delicate Mint DELM.

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 07-Jul-20Time: 11:35:32

Batch Name1 of 1

↑

BOOKING 1ST F3T18157 1-1 3018092/III/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 17-Apr-21Time: 10:36:55

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

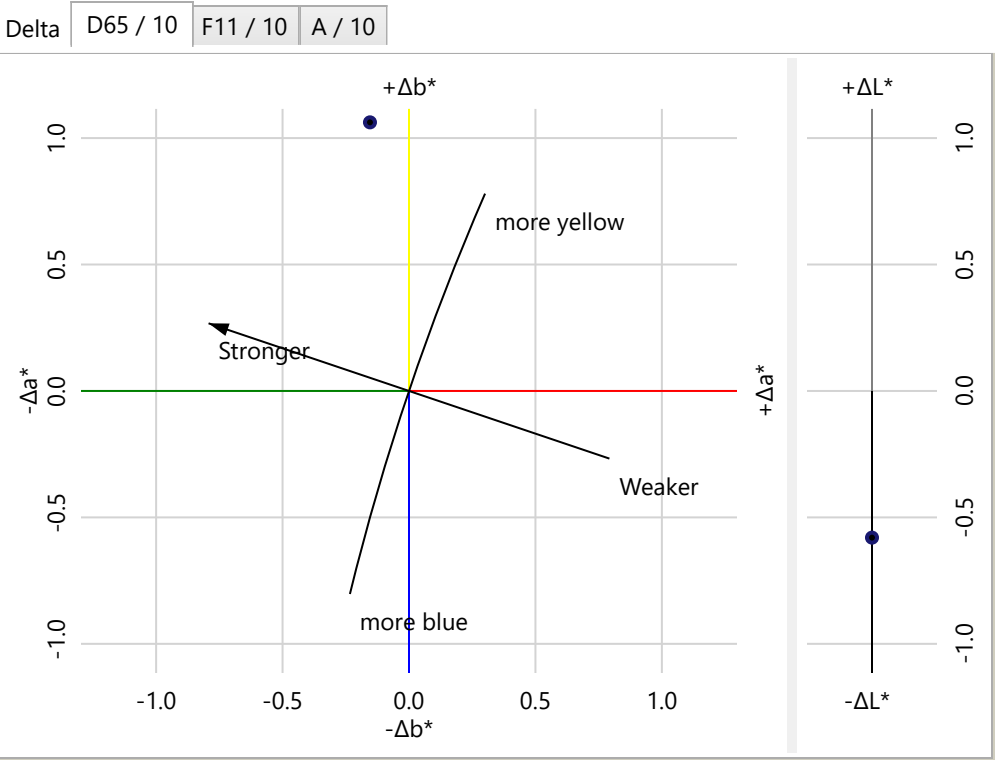

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
BOOKING 1ST F3T18157 1-1 3018092/III/21	D65 10 Deg	-0.58	-0.15	1.06	-0.21	0.44	-1.02	1.13		Fail	darker	more saturated more yellow
BOOKING 1ST F3T18157 1-1 3018092/III/21	F11 10 Deg	-0.09	-1.30	1.67	-0.03	1.55	-1.22	1.97	1.39	Fail	darker	more saturated more yellow
BOOKING 1ST F3T18157 1-1 3018092/III/21	A 10 Deg	-0.53	-1.79	1.38	-0.19	1.90	-1.14	2.23	1.67	Fail	darker	more saturated more yellow