

Standard Name 80 of 102

↑

Black 001 nOSC U01

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:Keyboard %R-40

Date: 18-Mar-21 Time: 02:52:00

Batch Name 2 of 7

↑

DKI18362 FZDM1AV/TVN1343 78-70 3005845/II

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 18-May-21 Time: 13:12:07

CMC DE Pass/Fail Tolerance: 1.00


I:c Ratio: ( 2.00 1.00)

Delta 

D65 / 10

U3500 / 10

A / 10

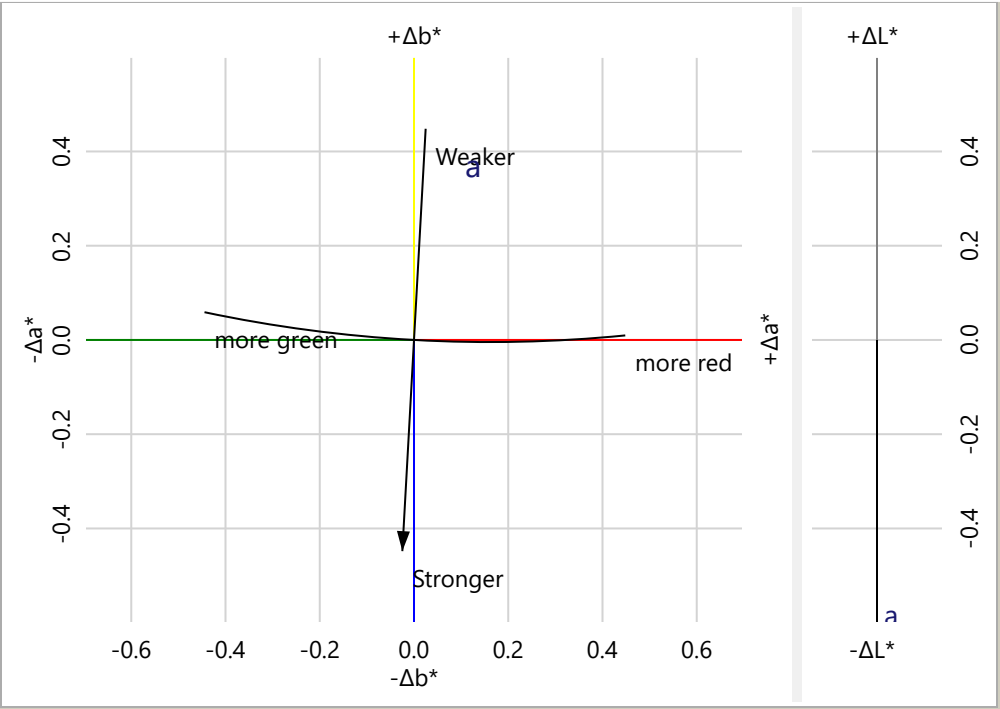

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
DKI18362 FZDM1AV/TVN1343 78-70 3005845/II/21	D65 10 Deg	-0.57	0.12	0.38	-0.52	-0.47	0.14	0.72		Pass	darker	less saturated more red
DKI18362 FZDM1AV/TVN1343 78-70 3005845/II/21	U3500 10 Deg	0.25	-0.01	0.82	-0.24	-0.91	-0.20	0.96	0.54	Warn	darker	less saturated more green
DKI18362 FZDM1AV/TVN1343 78-70 3005845/II/21	A 10 Deg	-0.57	-0.76	0.48	-0.52	-0.70	-0.90	1.26	0.88	Fail	darker	less saturated more green