

Standard Name 67 of 67

↑

GREY SAGE GRSG

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 04-Apr-18 Time: 08:54:59

Batch Name 1 of 1

↑

BKJFA21 MTR17080 75-28 3001793/I/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 27-Mar-21 Time: 14:48:07

CMC DE Pass/Fail Tolerance: 1.00


I:c Ratio: (2.00 1.00)

Delta

D65 / 10

F11 / 10

A / 10

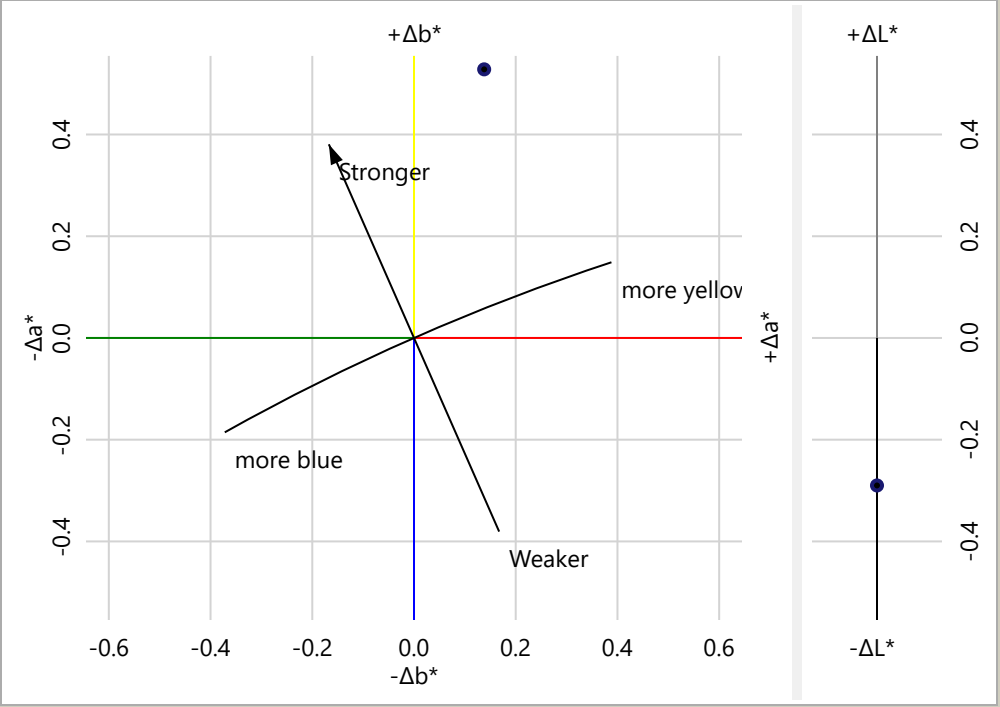

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments
BKJFA21 MTR17080 75-28 3001793/I/21	D65 10 Deg	-0.29	0.14	0.53	-0.15	0.49	-0.41	0.66		Pass	darker more saturated more yellow
BKJFA21 MTR17080 75-28 3001793/I/21	F11 10 Deg	-0.33	-0.52	0.89	-0.17	1.14	0.18	1.17	0.75	Fail	darker more saturated more blue
BKJFA21 MTR17080 75-28 3001793/I/21	A 10 Deg	-0.22	0.54	0.31	-0.11	0.40	-0.68	0.80	0.48	Warn	darker more saturated more red