

Standard Name58 of 67

↑

Gold Spice GLSC

↓

Visual Hue Request:

New StdRetrieve StdStore StdList StdUpdate Std

Instrument Setup:%R LAV SCI UV 400

Date: 18-Oct-20Time: 07:59:42

Batch Name1 of 1

↑

B21112905AA-003 MTR17080 1-1 3010907/II/21

↓

New BatRetrieve BatStore BatList BatUpdate Bat


Instrument Setup: %R LAV SCI UV Cal

Date: 27-Mar-21Time: 13:11:42

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

DeltaD65 / 10F11 / 10A / 10

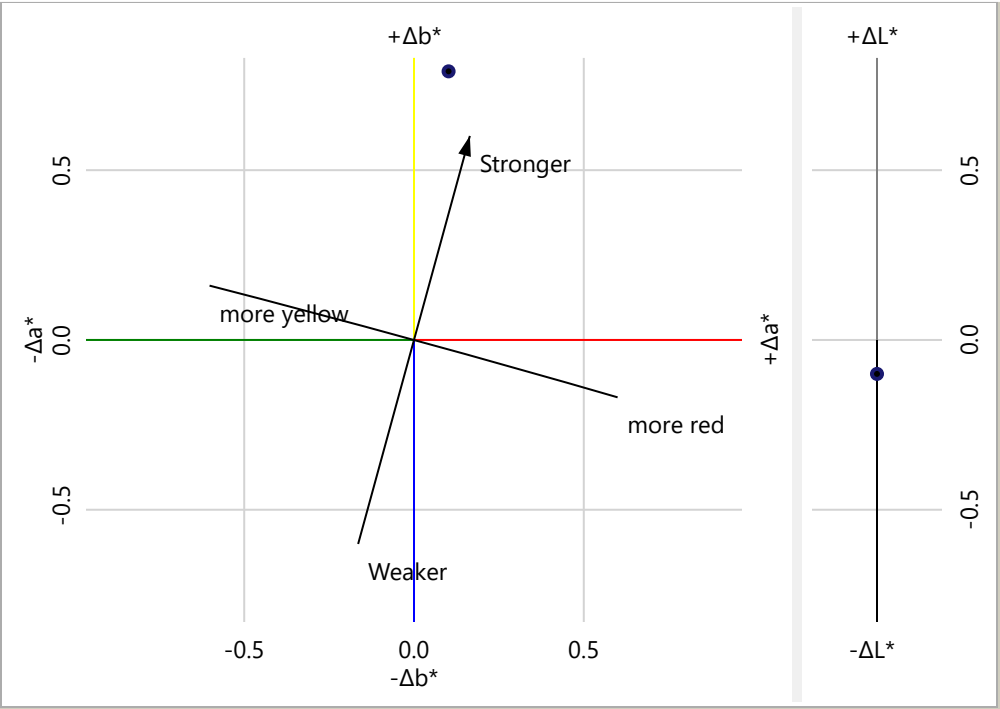

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
B21112905AA-003 MTR17080 1-1 3010907/II/21	D65 10 Deg	-0.09	0.10	0.78	-0.05	0.33	0.10	0.35		Pass	darker	more saturated more yellow
B21112905AA-003 MTR17080 1-1 3010907/II/21	F11 10 Deg	0.14	-0.18	1.08	0.07	0.43	0.25	0.50	0.48	Pass	lighter	more saturated more green
B21112905AA-003 MTR17080 1-1 3010907/II/21	A 10 Deg	-0.09	-0.93	0.95	-0.04	0.25	1.00	1.03	1.04	Fail	darker	more saturated more yellow