

Standard Name216 of 216

↑

5A 0560 C /FBM15042(FLT)/BLACK(09)/STD MI

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 09-Aug-18Time: 20:40:50

Batch Name2 of 2

↑

FA21-ITN-B107&B108 FBM15293 3-1 3015862.1

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 08-Apr-21Time: 14:57:38

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: ( 2.00 1.00)

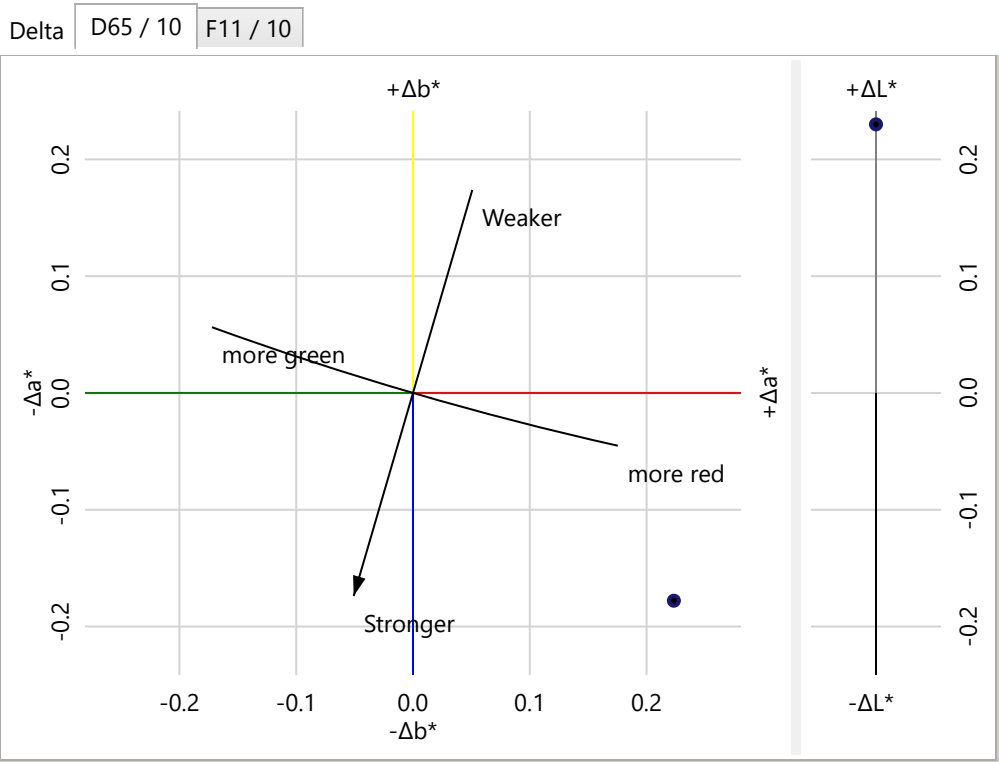

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments
FA21-ITN-B107&B108 FBM15293 3-1 3015862.3015961/II	D65 10 Deg	0.23	0.22	-0.18	0.21	0.14	0.34	0.43		Pass	lighter more saturated more red
FA21-ITN-B107&B108 FBM15293 3-1 3015862.3015961/II	F11 10 Deg	0.39	0.26	-0.05	0.37	-0.06	0.33	0.50	0.21	Pass	lighter less saturated more red