

Standard Name 43 of 113

↑

18157/220306D-A

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV SCI UV Cal

Date: 27-May-22 Time: 14:33:47

Batch Name 3 of 4

↑

B22209901AA-001 1-1K1 3059663/X/22KELLY G

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal


Date: 29-Nov-22 Time: 13:35:16

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments		
R1117235 B22209901AA-001 1-1K1 3059663/X/22KELLY G	D65 10 Deg	0.03	0.42	-0.72	0.01	-0.21	0.34	0.39		Pass	too light	too dull	too blue
R1117235 B22209901AA-001 1-1K1 3059663/X/22KELLY G	F11 10 Deg	-0.08	0.90	-0.92	-0.04	-0.43	0.44	0.62	0.54	Pass	too dark	too dull	too blue
R1117235 B22209901AA-001 1-1K1 3059663/X/22KELLY G	A 10 Deg	0.01	0.56	-0.75	0.00	-0.20	0.42	0.47	0.17	Pass	too light	too dull	too blue

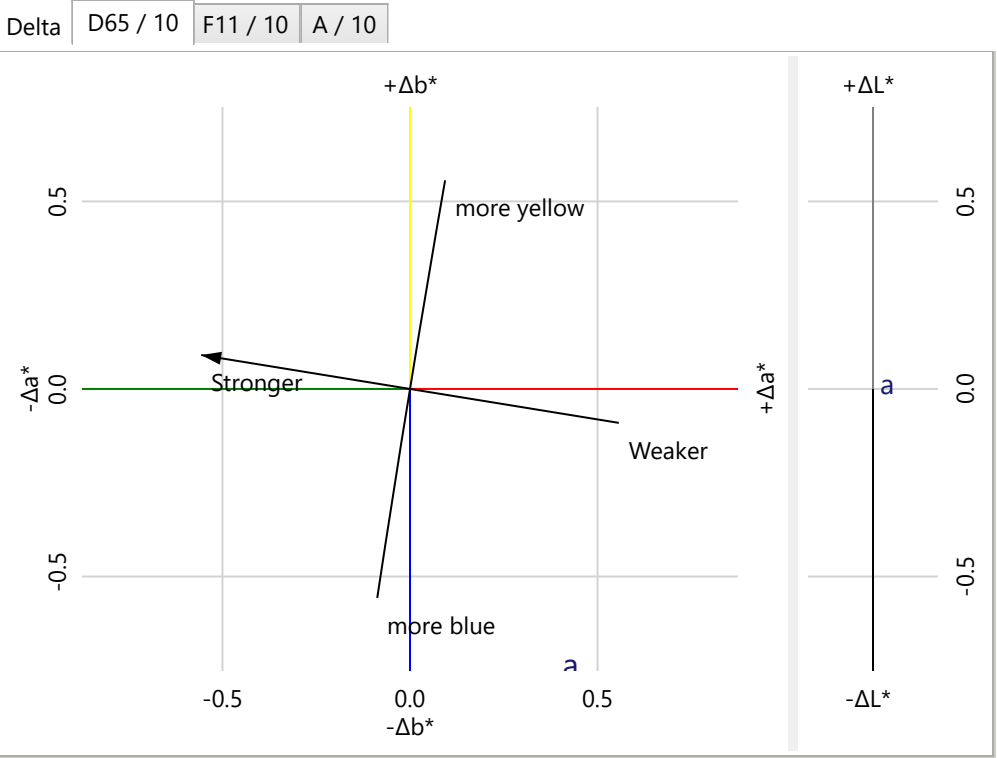

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form