

Standard Name 88 of 88

↑

8A 0395-4 FSC

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV 400

Date: 31-Oct-18 Time: 13:15:46

Batch Name 1 of 1

↑

FA21-ITN-B104 SJS18232 3-1 3012710/II/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 27-May-21 Time: 15:38:13


CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: ( 2.00 1.00)

Delta 

D65 / 10

F11 / 10

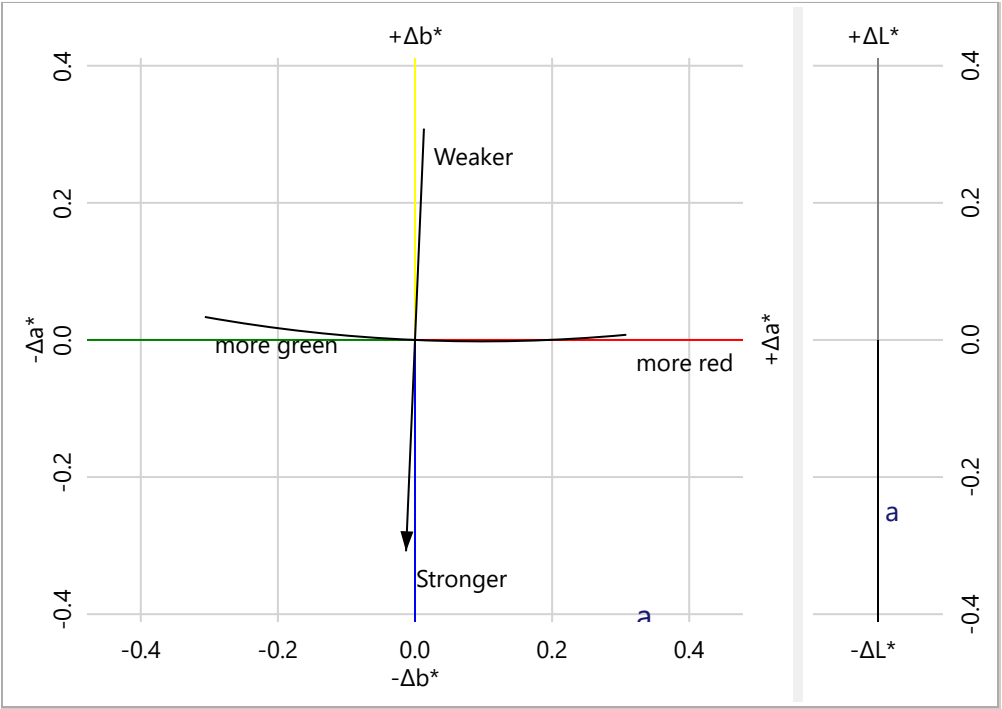

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
FA21-ITN-B104 SJS18232 3-1 3012710/II/21	D65 10 Deg	-0.24	0.33	-0.39	-0.20	0.51	0.43	0.70		Warn	darker	more saturated more red
FA21-ITN-B104 SJS18232 3-1 3012710/II/21	F11 10 Deg	-0.04	0.13	-0.16	-0.04	0.15	0.22	0.26	0.37	Pass	darker	more saturated more red