

Standard Name 169 of 169

21B 0347 CRD

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal

Date: 26-Aug-21 Time: 16:44:48

Batch Name 1 of 3

↑
F3C17109 PR2122/68716 6-1 3052636/VII/21
↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal

Date: 15-Sep-21 Time: 13:28:35

CMC DE Pass/Fail Tolerance: 1.00


I:c Ratio: (2.00 1.00)

Measured by: ▼

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/F	Color	Comments	
F3C17109 PR2122/68716 6-1 3052636/VII/21	D65 10 Deg	-0.46	0.24	-0.58	-0.23	0.28	0.38	0.53		Pass	too dark	too bright	too red
F3C17109 PR2122/68716 6-1 3052636/VII/21	F11 10 Deg	-0.56	0.31	-0.72	-0.29	0.35	0.41	0.61	0.23	Pass	too dark	too bright	too red
F3C17109 PR2122/68716 6-1 3052636/VII/21	A 10 Deg	-0.49	0.37	-0.64	-0.26	0.24	0.47	0.59	0.15	Pass	too dark	too bright	too red

DataColor TOOLS 2.8.1

S/N NO. 8823242

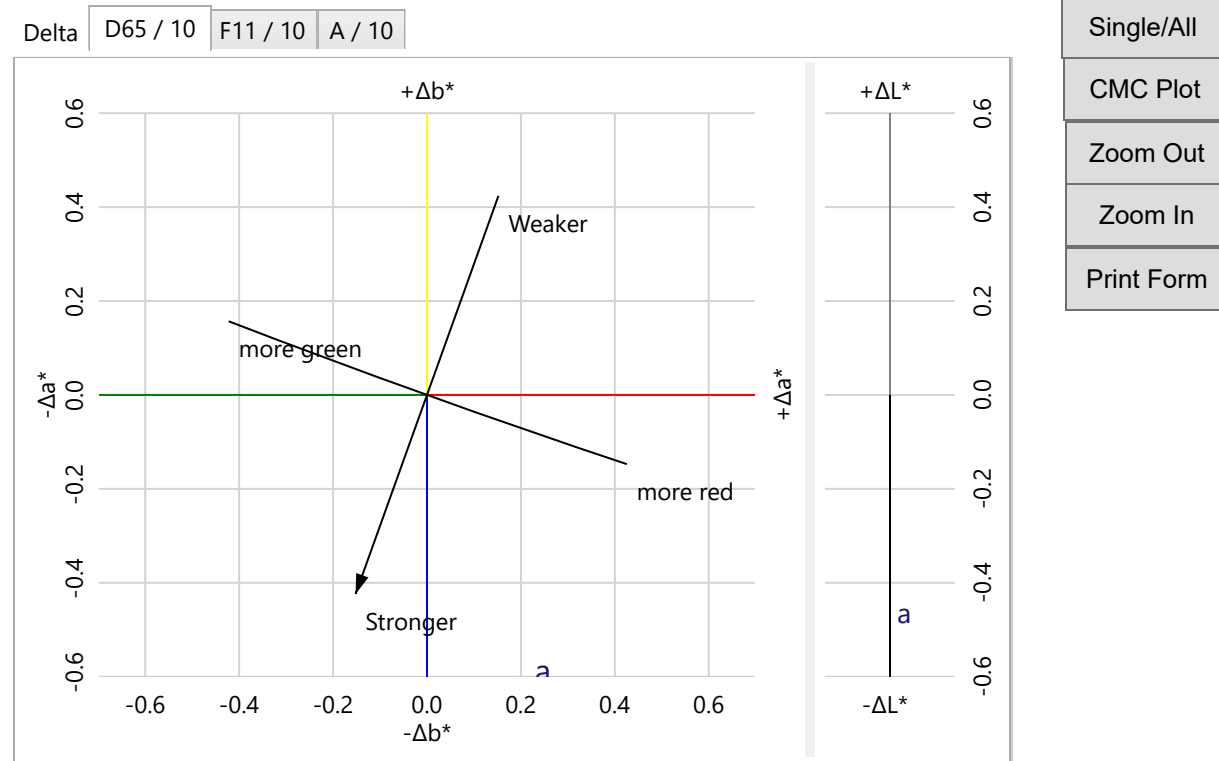

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form