

Standard Name105 of 105

↑

9C 1086-1 BRM

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal
Date: 17-Dec-19Time: 09:43:30

Batch Name1 of 1

↑

BKJ FA21 F3T18157 5-3/K2 3001793/I/21

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal
Date: 26-Apr-21Time: 14:41:16

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

DeltaD65 / 10F11 / 10A / 10

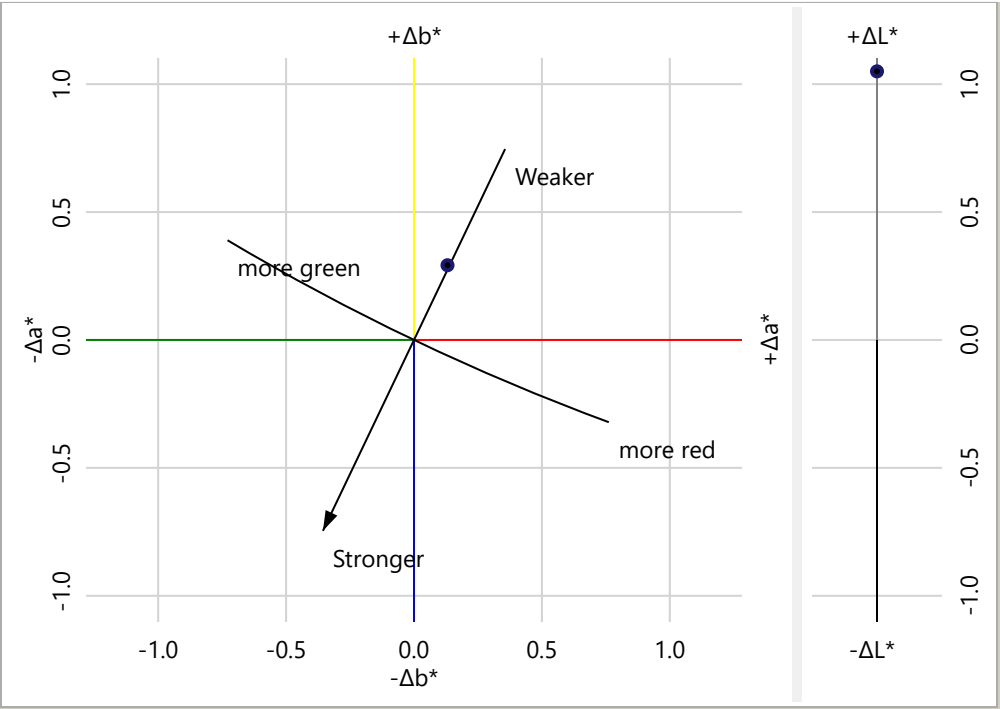

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments
BKJ FA21 F3T18157 5-3/K2 3001793/I/21	D65 10 Deg	1.06	0.13	0.29	0.45	-0.27	-0.01	0.53		Pass	lighter	less saturated more green
BKJ FA21 F3T18157 5-3/K2 3001793/I/21	F11 10 Deg	1.18	0.02	0.47	0.51	-0.37	-0.15	0.65	0.27	Pass	lighter	less saturated more green
BKJ FA21 F3T18157 5-3/K2 3001793/I/21	A 10 Deg	1.09	0.03	0.37	0.47	-0.29	-0.13	0.57	0.15	Pass	lighter	less saturated more green