

Standard Name 69 of 69

↑

9A 0568 ASC

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 10-Oct-19 Time: 16:04:51

Batch Name 2 of 2

↑

1-ITN-B106 SJS18232 1-1 3055122/VIII/21 GR1

↓

New Bat

Retrieve Bat

Store Bat

List Bat


Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 24-Aug-21 Time: 15:07:52

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: ( 2.00 1.00)

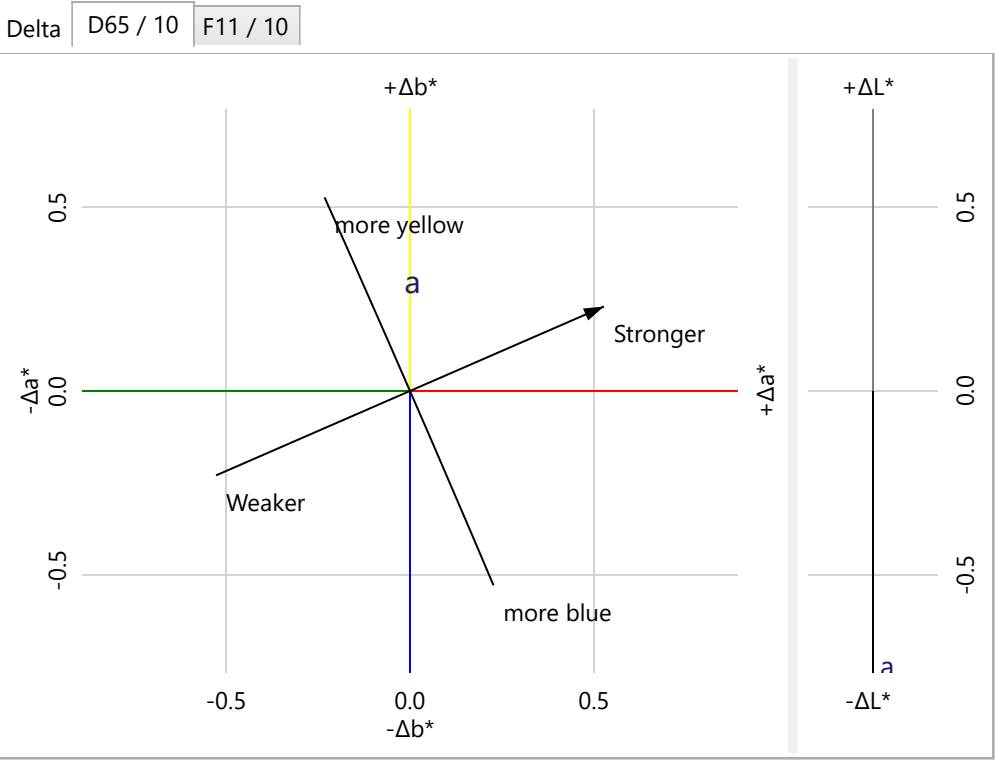

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments		
FA21-ITN-B106 SJS18232 1-1 3055122/VIII/21 GR1	D65 10 Deg	-0.73	-0.00	0.32	-0.38	0.05	0.19	0.43		Pass	too dark	too bright	too yellow
FA21-ITN-B106 SJS18232 1-1 3055122/VIII/21 GR1	F11 10 Deg	-0.72	-0.10	0.40	-0.36	0.04	0.28	0.46	0.24	Pass	too dark	too bright	too yellow