

Standard Name139 of 159

↑

20124/220356S-A

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 20-Jun-22Time: 13:47:24

Batch Name1 of 2

↑

1741911 53674 EXP2300153 COLLEGE COBAL

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal


Date: 16-Mar-23Time: 14:45:48

CMC DE Pass/Fail Tolerance:1.00

I:c Ratio: (2.001.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
HJY20124 4501741911 53674 EXP2300153 COLLEGE COBAL D65 10 Deg		0.36	-0.45	0.56	0.26	-0.29	-0.25	0.46		Pass	too light	too dull	too green
HJY20124 4501741911 53674 EXP2300153 COLLEGE COBAL F11 10 Deg		0.49	-0.81	0.85	0.37	-0.40	-0.50	0.74	0.52	Pass	too light	too dull	too green
HJY20124 4501741911 53674 EXP2300153 COLLEGE COBAL A 10 Deg		0.41	-0.81	0.77	0.32	-0.29	-0.62	0.76	0.42	Warn	too light	too dull	too green

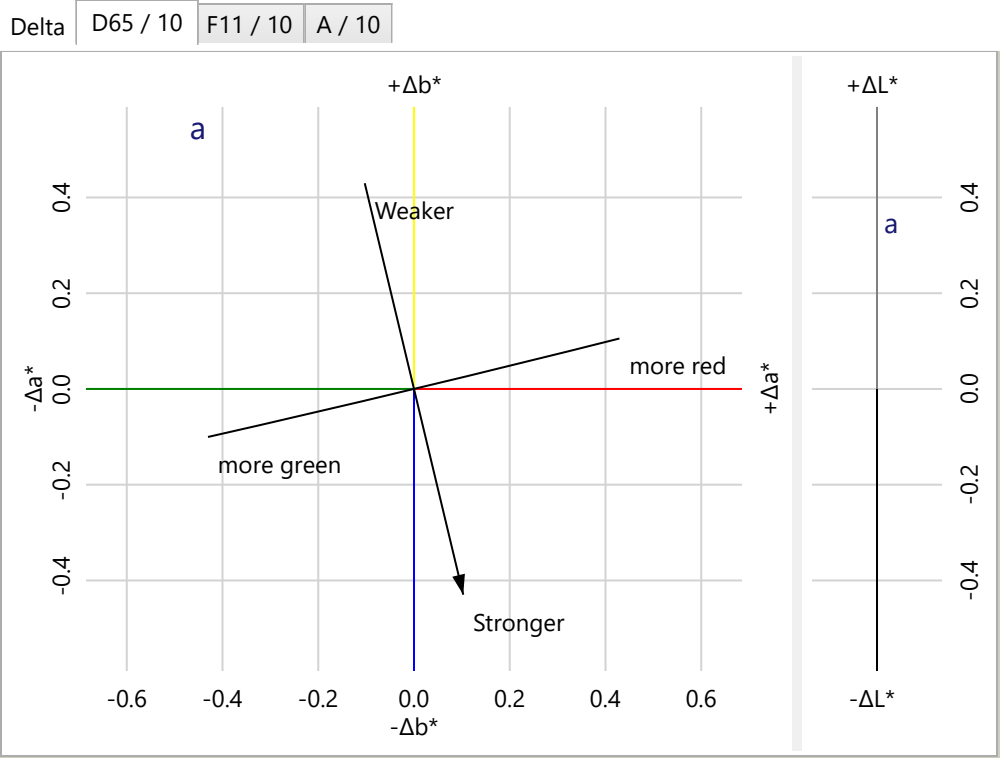

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form