


Instrument Setup: %R LAV SCI UV Cal
Date: 07-Feb-24 Time: 11:23:18

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

Measured by:

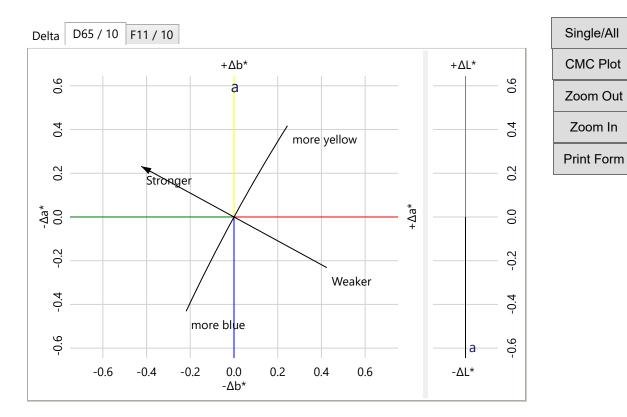

Batch Name III/Obs DL* <u>Da*</u> Db* DL*/ISL DC*/cSC DH*/SH CMC DE P/F **Color Comments** <u>M.I.</u> DKF19106 24050171IR-01 119019 EXP2400010 D65 10 Deg -0.58 0.61 -0.28 0.28 -0.60 0.72 too yellow Warn too dark too bright DKF19106 24050171IR-01 119019 EXP2400010 F11 10 Deg -0.55 0.10 0.70 -0.27 0.22 -0.74 0.81 Pass too dark too bright too yellow 0.13