

Standard Name 332 of 339

↑

7091/230024S-A

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 06-Feb-23 Time: 09:31:09

Batch Name 1 of 1

↑

3090114IR-02 72442 EXP2300369 DEEP LUXE

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal


Date: 05-Jul-23 Time: 13:18:59

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (1.50 2.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
SJS7091 23090114IR-02 72442 EXP2300369 DEEP LUXE	D65 10 Deg	0.07	0.64	-0.27	0.07	0.17	-0.17	0.25		Pass	too light	too bright	too blue
SJS7091 23090114IR-02 72442 EXP2300369 DEEP LUXE	F11 10 Deg	0.13	0.72	-0.21	0.12	0.19	-0.17	0.28	0.11	Pass	too light	too bright	too blue
SJS7091 23090114IR-02 72442 EXP2300369 DEEP LUXE	A 10 Deg	0.13	0.53	-0.14	0.11	0.13	-0.19	0.26	0.19	Pass	too light	too bright	too blue

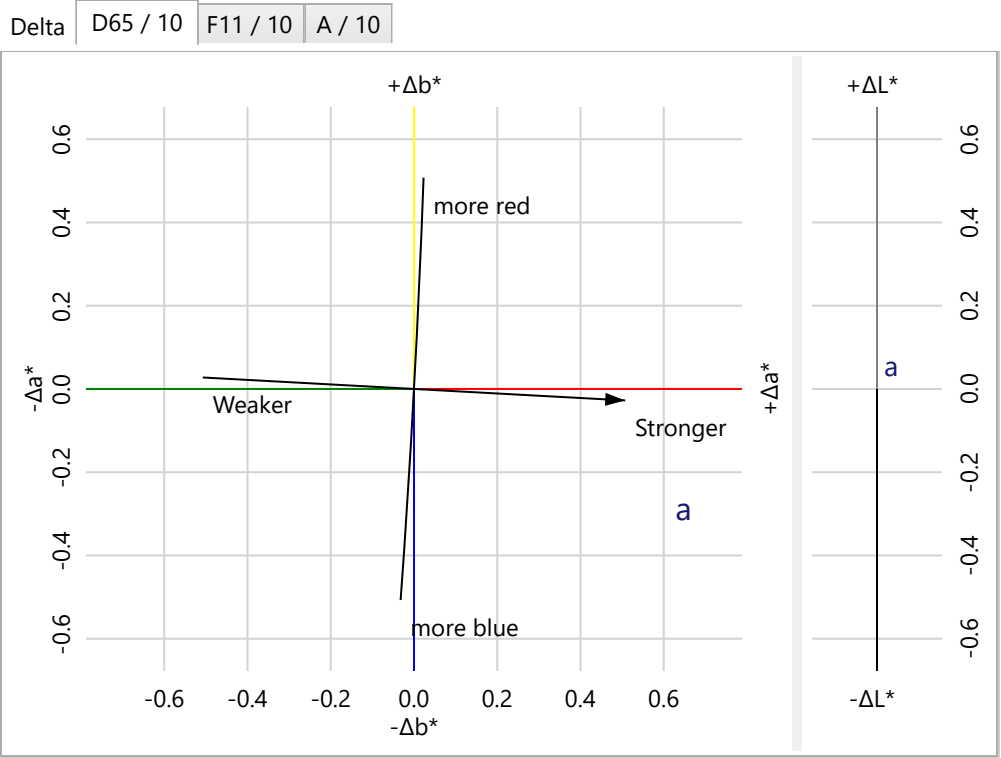

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form