

Standard Name 107 of 126

↑

19053/220471M-B

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 04-Aug-22 Time: 16:37:28

Batch Name 1 of 1

↑

53 5344802 54982 DOM2300106 PURPLE ASH

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal

Date: 26-Feb-23 Time: 14:27:14

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)


Measured by:

Delta

D65 / 10

F11 / 10

A / 10

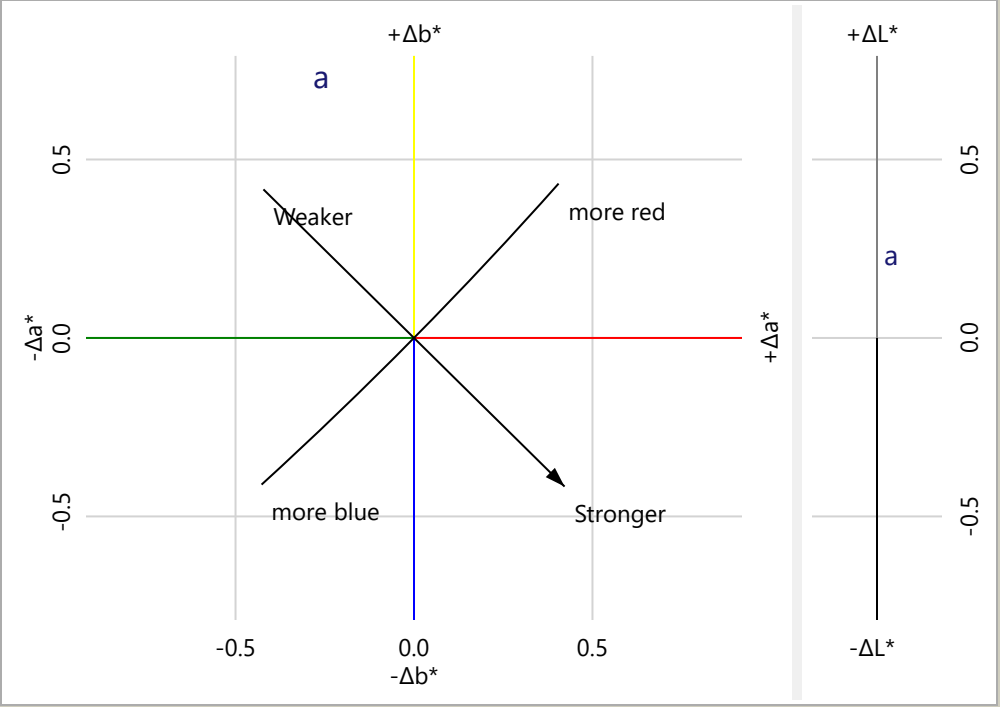

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

| Batch Name | III/Obs | DL* | Da* | Db* | DL*/ISL | DC*/cSC | DH*/SH | CMC DE | M.I. | P/E | Color | Comments | |
|--|------------|------|-------|------|---------|---------|--------|--------|------|------|-----------|----------|---------|
| SPQ19053 5344802 54982 DOM2300106 PURPLE ASH | D65 10 Deg | 0.25 | -0.26 | 0.76 | 0.12 | -0.56 | 0.42 | 0.71 | | Pass | too light | too dull | too red |
| SPQ19053 5344802 54982 DOM2300106 PURPLE ASH | F11 10 Deg | 0.31 | -0.12 | 0.91 | 0.15 | -0.61 | 0.57 | 0.85 | 0.22 | Warn | too light | too dull | too red |
| SPQ19053 5344802 54982 DOM2300106 PURPLE ASH | A 10 Deg | 0.27 | -0.14 | 0.76 | 0.13 | -0.50 | 0.57 | 0.77 | 0.13 | Warn | too light | too dull | too red |